


HPLC COLUMN TEST SUMMARY

| | | | |
|-------------------|----------------------|-------------------|---------------|
| Catalog No: | HP-B02-2105 | Mobile Phase: | ACN:H2O=70:30 |
| Serial No: | H22032101 | Flow Rate: | 0.2ml/min |
| Batch No: | H2201A | Temperature: | Ambient |
| Stationary Phase: | Hungpu C18 2 μ m | Detector: | 254nm |
| Dimensions: | 50*2.1mm | Injection Volume: | 0.2 μ l |
| Pressure: | 1361psi | Sample: | toluene |

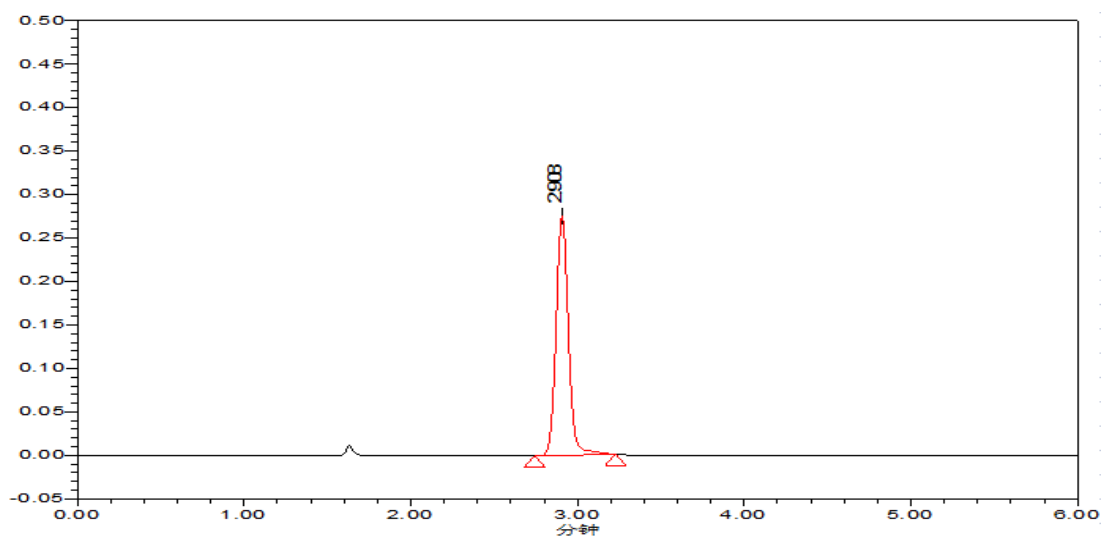

| Item | Sample | Ret Time (min) | USP Tailing (As) | Efficiency (N/m) |
|------|---------|-------------------|---------------------|---------------------|
| 1 | toluene | 2.908 | 1.07 | 7364.58 |

Test Result: Qualified