


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-B02-2105	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22032103	Flow Rate:	0.2ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu C18 2 $\mu$ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	0.2 $\mu$ l
Pressure:	1362psi	Sample:	toluene

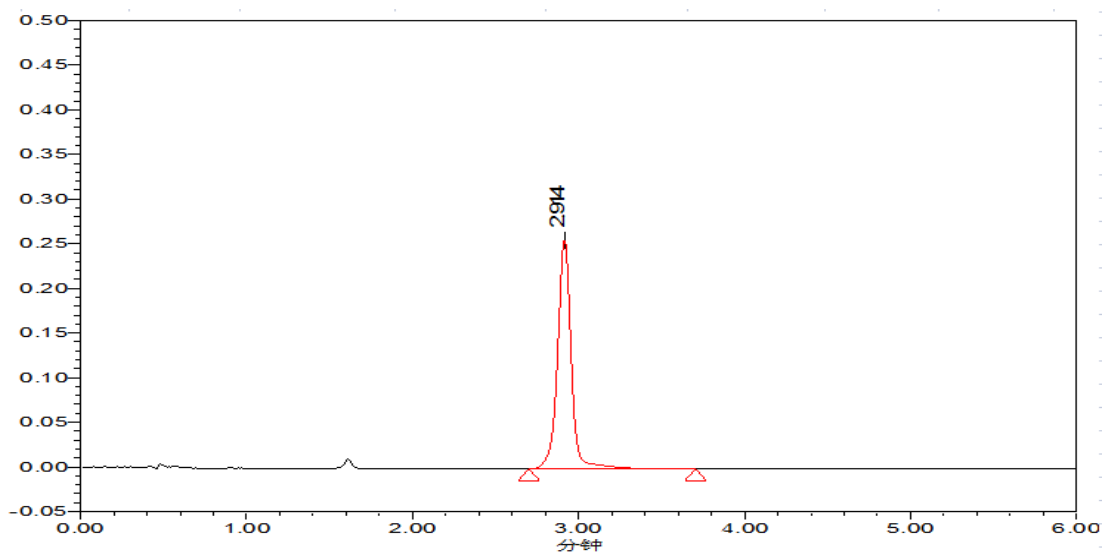

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	toluene	2.914	0.95	7351.21

Test Result: Qualified