


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-0315	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22030501	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu C18-AQ(2) 3 μ m	Detector:	254nm
Dimensions:	150*3.0mm	Injection Volume:	20 μ l
Pressure:	171bar	Sample:	Toluene

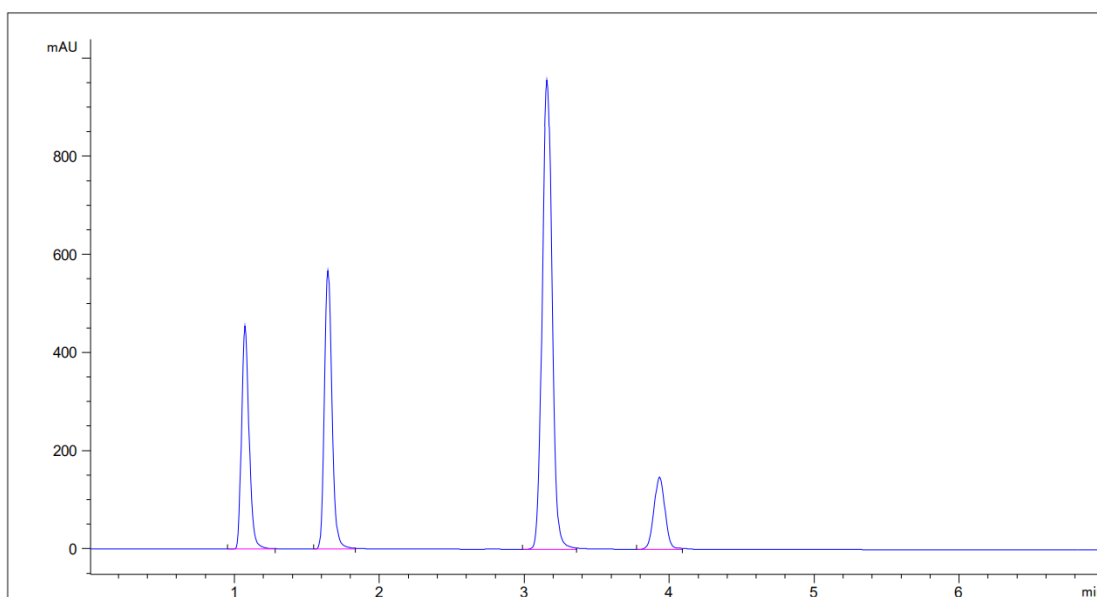

Item	Sample	Ret Time(min)	USP Tailing	Efficiency
1	Toluene	3.676	0.99	12330

Test Result: Qualified