


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-DH05-4625	Mobile Phase:	n-hexane :isopropanol =99.5:0.5
Serial No:	H22032301	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu DIOL-HILIC 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	20 μ l
Pressure:	29bar	Sample:	Nitrobenzene

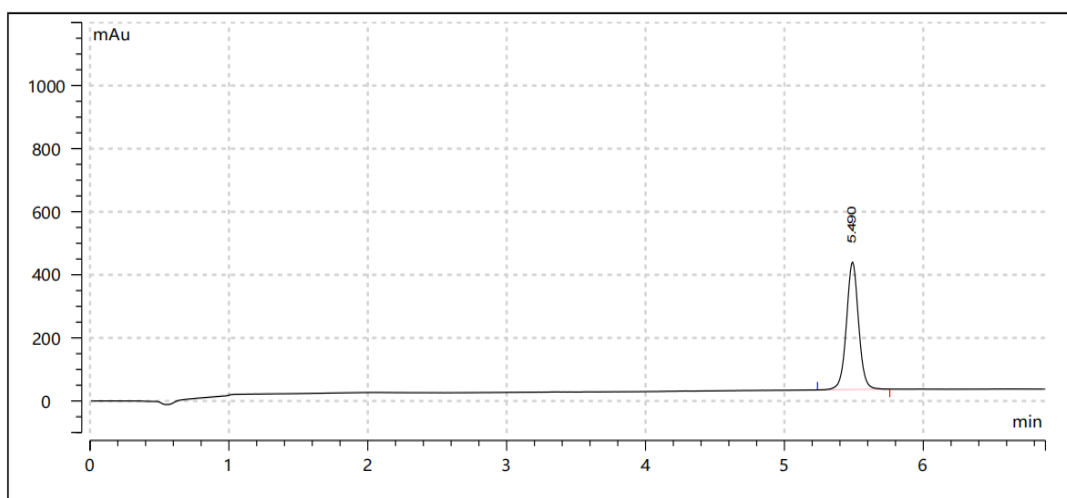

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Nitrobenzene	5.49	1.02	20180

Test Result:Qualified