


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BS05-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22030605	Flow Rate:	1.0ml/min
Batch No:	S02050-J01-011002	Temperature:	Ambient
Stationary Phase:	Hungpu ST C18 5μm	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5μl
Pressure:	7.8Mpa	Sample:	Uracil 、 Acetone、 Acenaphthene

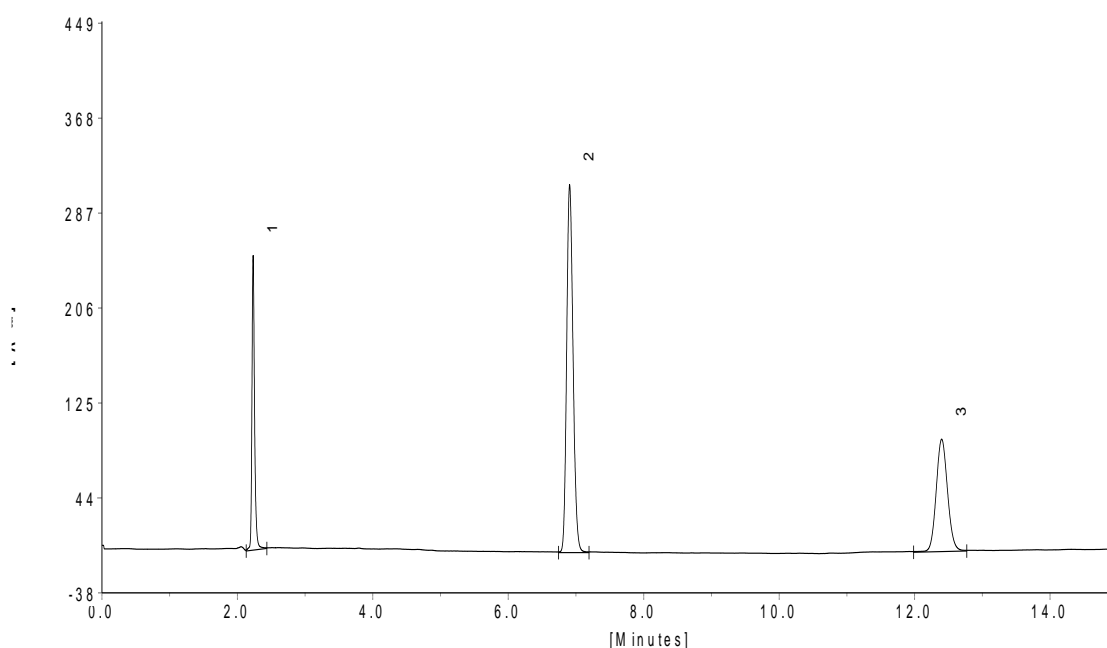

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Uracil	2.23	1.31	75162
2	Toluene	6.90	1.17	93942
3	Acenaphthene	12.40	1.09	108147

Test Result:Qualified