


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX05-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22030604	Flow Rate:	0.8ml/min
Batch No:	H02050-J06-011004	Temperature:	Ambient
Stationary Phase	Hungpu XBT C18 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5 μ l
Pressure:	5.9Mpa	Sample:	Acetone、Acenaphthene

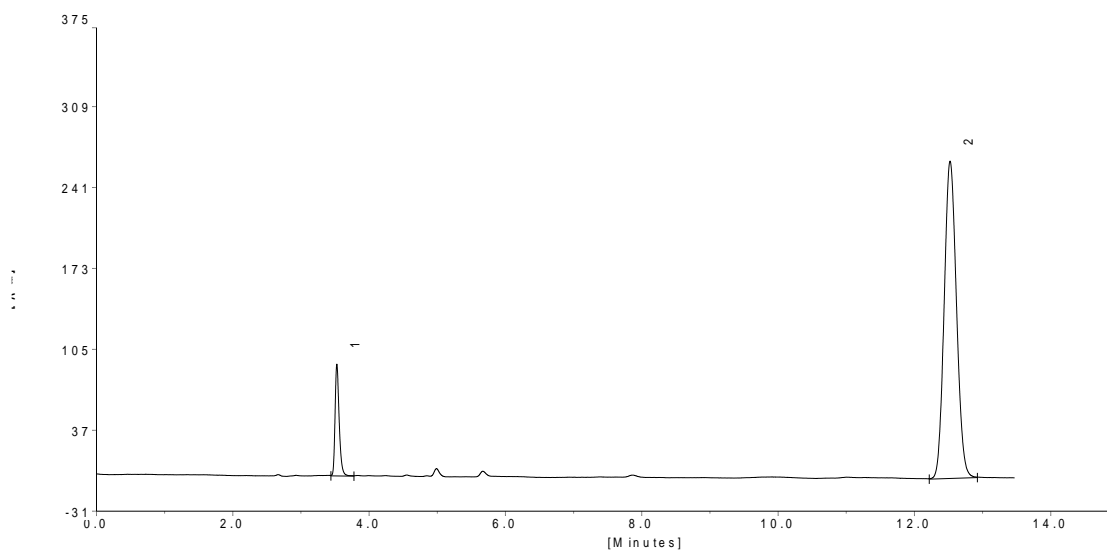

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	3.52	1.35	68679
2	Acenaphthene	12.52	1.09	91410

Test Result:Qualified