


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX05-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H21101701	Flow Rate:	0.8ml/min
Batch No:	H011003-01100089	Temperature:	Ambient
Stationary Phase:	Hungpu XBT C18 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5 μ m
Pressure:	5.5Mpa	Sample:	Uracil 、Toluene、Acenaphthene

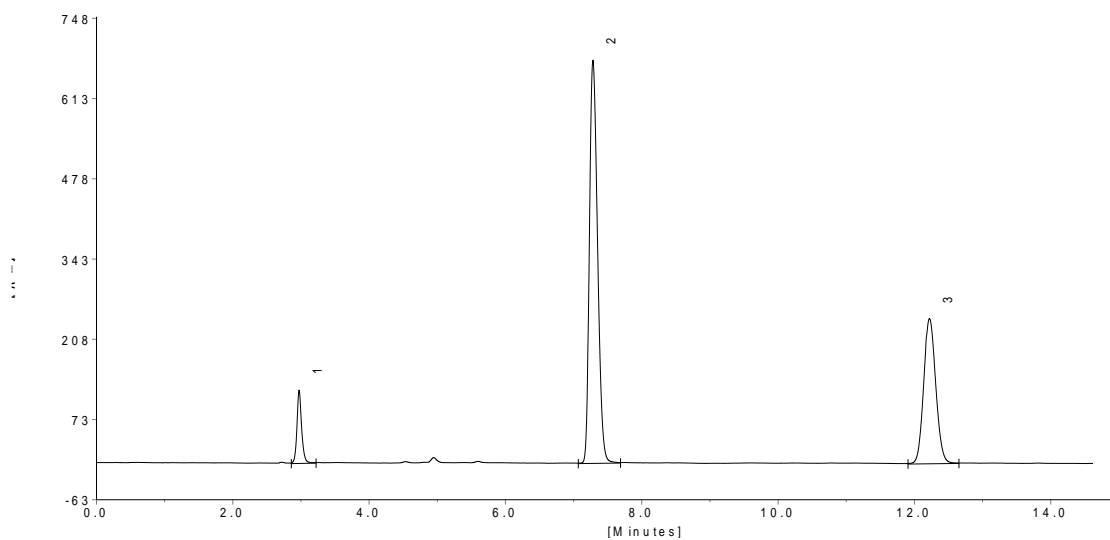

Item	Sample	Ret Time (min)	Capacity Factor	USP Tailing (As)	Efficiency (N/m)
1	Uracil	2.97	0.00	1.16	42974
2	Toluene	7.28	1.45	1.26	70457
3	Acenaphthene	12.22	3.11	1.09	91690

Test Result:Qualified