


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX05-2025	Mobile Phase:	ACN:H2O=60:40
Serial No:	H22032604	Flow Rate:	16ml/min
Batch No:	H02050-J06-011005	Temperature:	Ambient
Stationary Phase	Hungpu XBT C18 5 μ m	Detector:	254nm
Dimensions:	250*20mm	Injection Volume:	20 μ l
Pressure:	9.3Mpa	Sample:	Uracil/Acetophenone/ Toluene/Ethylbenzene /Fluorene

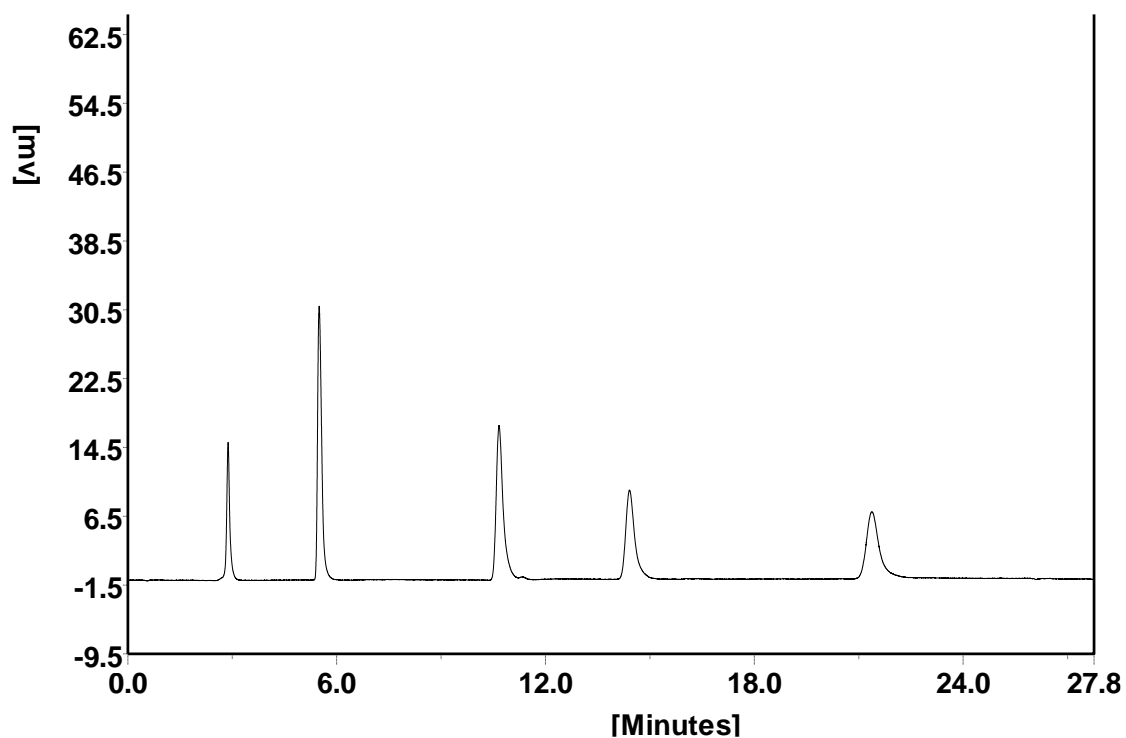

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Uracil	2.88	1.29	27000
2	Acetophenone	5.50	1.55	43400
3	Toluene	10.66	1.54	66800
4	Ethylbenzene	14.41	1.51	68900
5	Fluorene	21.37	1.30	77300

Test Result: Qualified