


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-A05-4625	Mobile Phase:	100 mM ammonium formate PH3.2:ACN=15:85
Serial No:	H22032602	Flow Rate:	0.6ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu Amide 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	20 μ l
Pressure:	39bar	Sample:	Cytosine

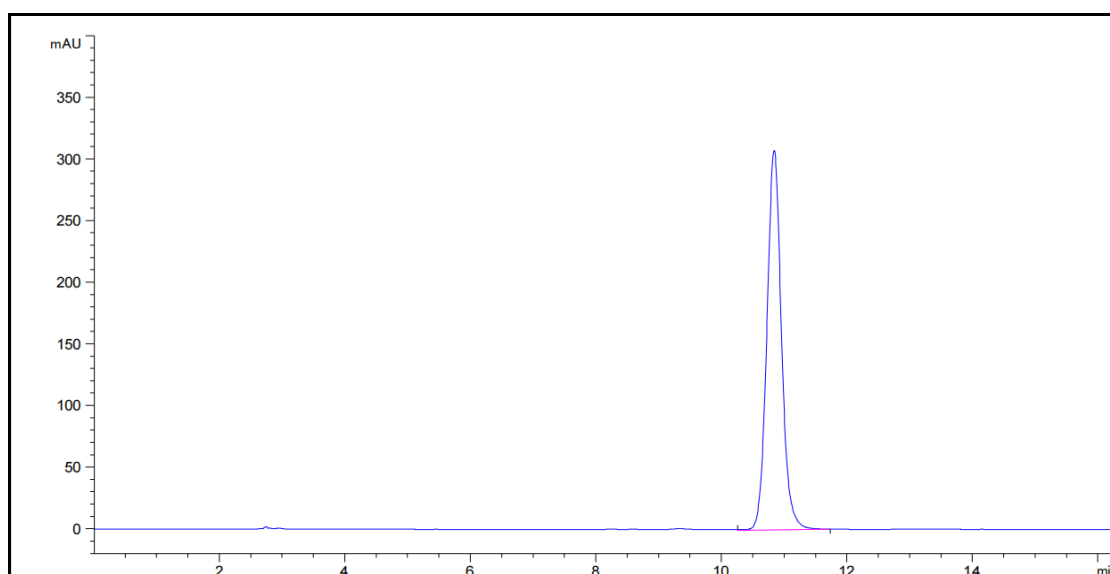

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Cytosine	10.921	1.06	17742

Test Result: Qualified