


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-H08-7830	Mobile Phase:	H ₂ SO ₄ in Water (pH=2.5)
Serial No:	H22040501	Flow Rate:	0.6ml/min
Batch No:	H2201A	Temperature:	55 °C
Stationary Phase	Hungpu Sugar-H 8μm	Detector:	207nm
Dimensions:	300*7.8mm	Injection Volume:	20μl
Pressure:	30bar	Sample:	Ribavirin

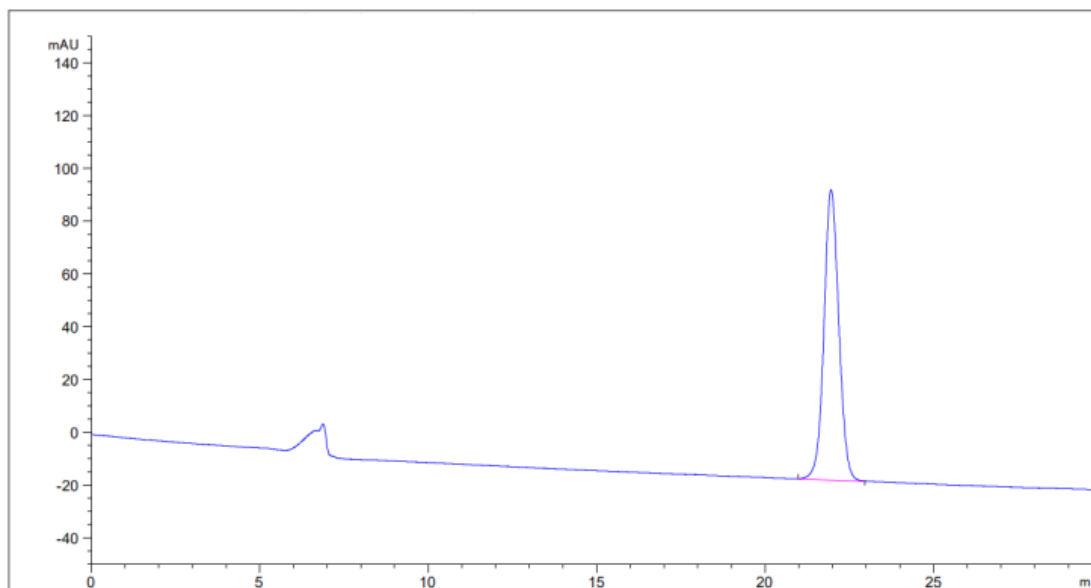

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Ribavirin	21.96	1.09	13000

Test Result: Qualified

