


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-2105	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22040601	Flow Rate:	0.2ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase	Hungpu C18-AQ(2) 3μm	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	0.2μl
Pressure:	44bar	Sample:	Naphthalene

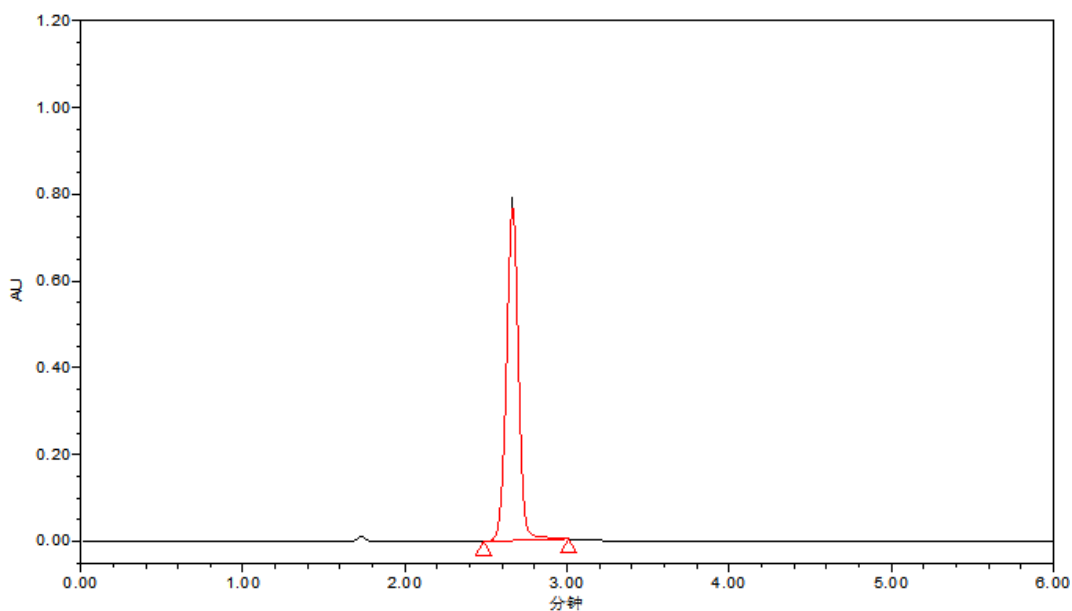

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Naphthalene	2.664	0.98	6365

Test Result: Qualified

