


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-0315	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22052002	Flow Rate:	0.6ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ(2) 3μm	Detector:	254nm
Dimensions:	150*3.0mm	Injection Volume:	3μl
Pressure:	145bar	Sample:	Fluorene

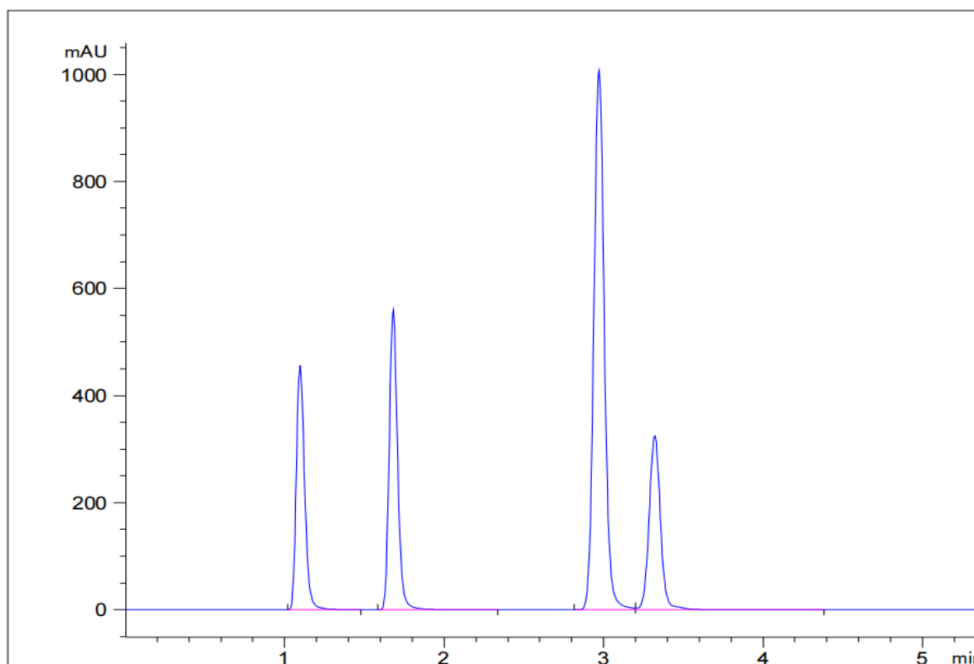

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Fluorene	3.321	1.02	11028

Test Result: Qualified

