


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y05-4625	Mobile Phase:	MeOH:H2O=75:25
Serial No:	H22052001	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ(2) 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	20 μ l
Pressure:	130bar	Sample:	Toluene

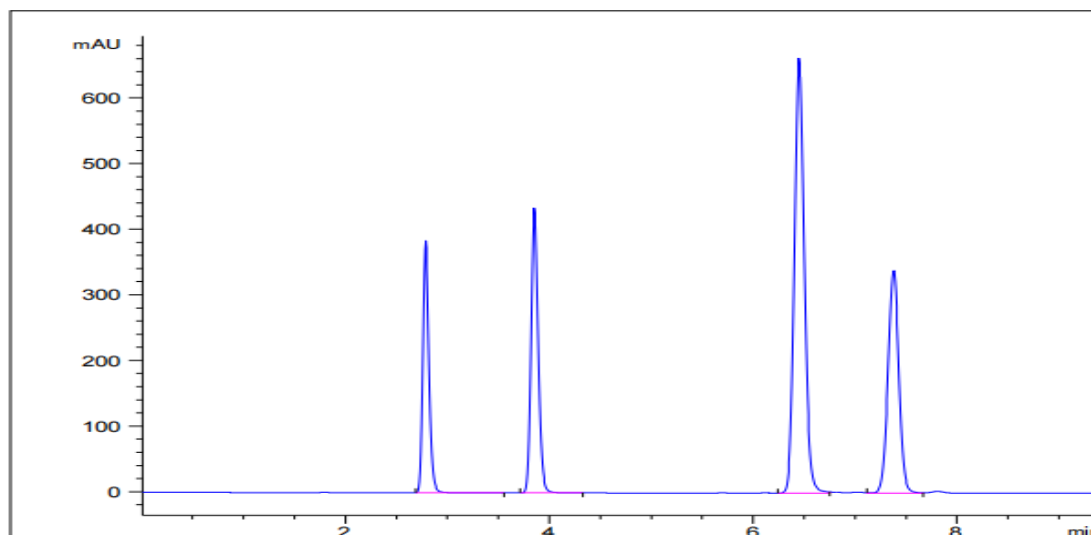

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	7.369	0.99	23375

Test Result: Qualified

