


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-WT05-1025	Mobile Phase:	ACN:H2O=60:40
Serial No:	H22050801	Flow Rate:	4ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu C4-300 5 μ m	Detector:	254nm
Dimensions:	250*10mm	Injection Volume:	20 μ l
Pressure:	89bar	Sample:	Toluene

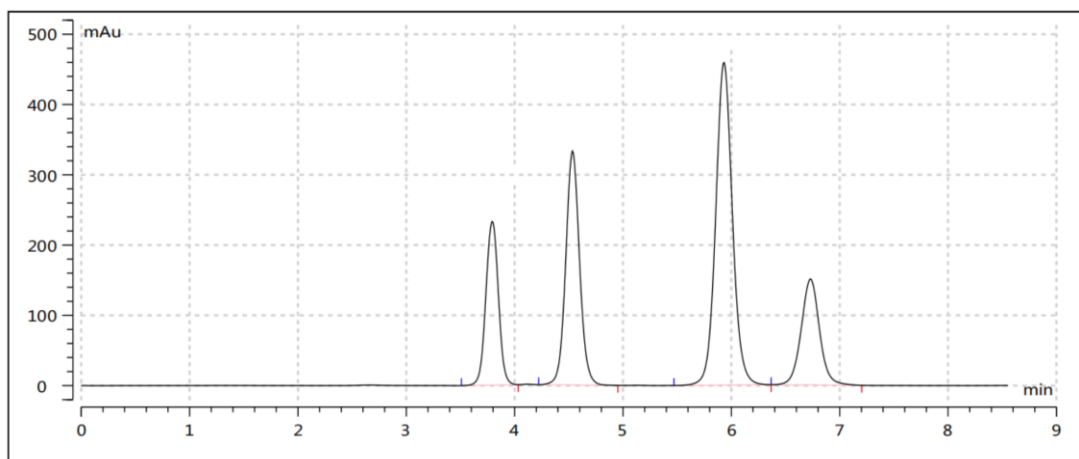

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	6.733	1.22	21996

Test Result: Qualified

