


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-C05-4625	Mobile Phase:	MeOH:H <sub>2</sub> O=75:25
Serial No:	H22050110	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu C8 5μm	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	20μl
Pressure:	137bar	Sample:	Toluene

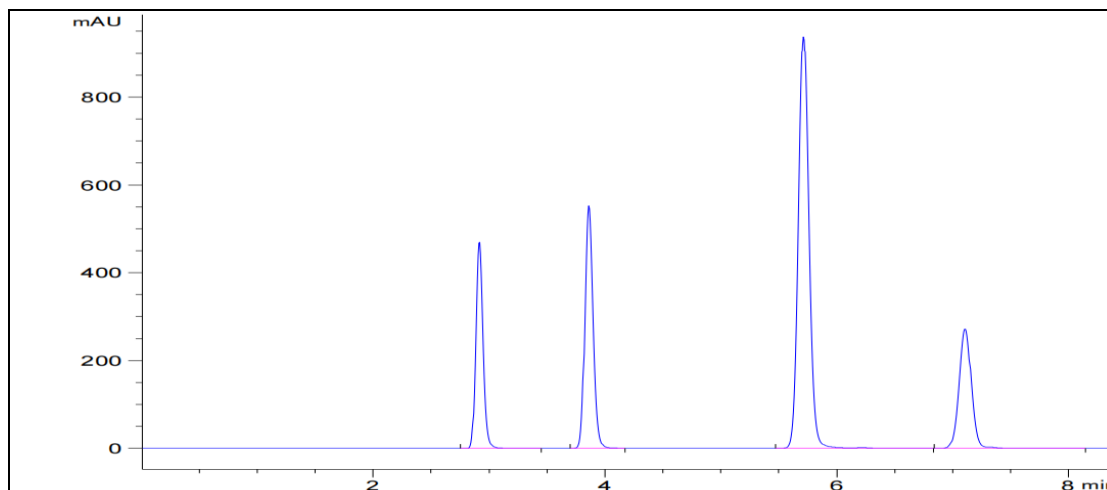

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	7.110	0.99	21891

Test Result: Qualified

