


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-J05-4612.5	Mobile Phase:	ACN:H2O=30:70
Serial No:	H22041704	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu CN 5 μ m	Detector:	254nm
Dimensions:	100*4.6mm	Injection Volume:	10 μ l
Pressure:	51bar	Sample:	Nitrobenzene

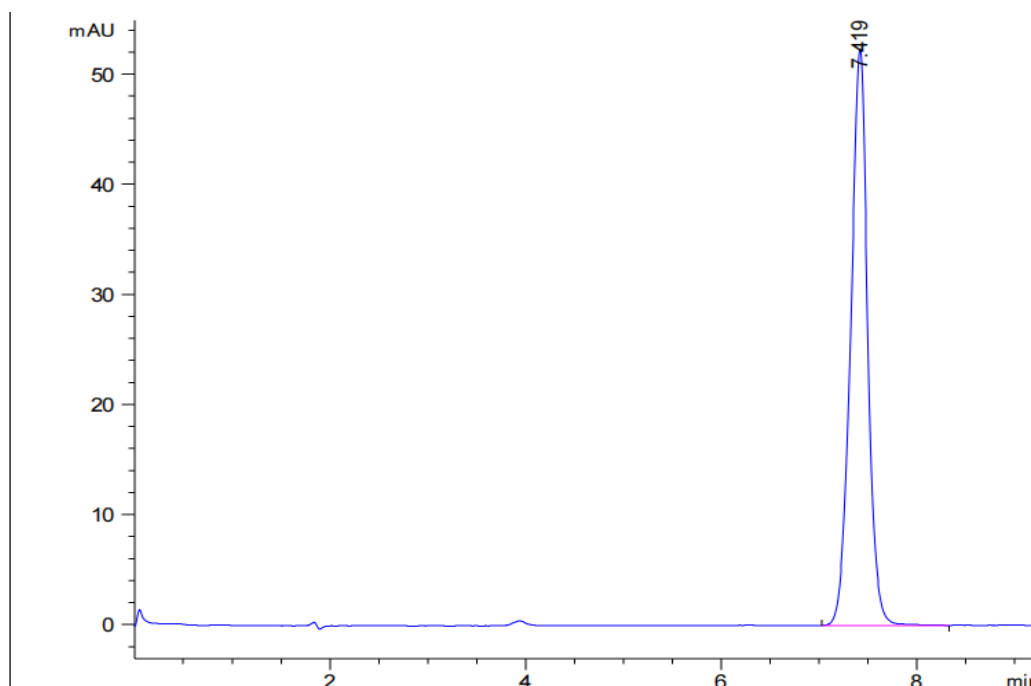

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Nitrobenzene	7.419	1.06	8006

Test Result: Qualified

