


HPLC COLUMN TEST SUMMARY

Test Column :	Hungu Ghost-Caputurer 50*4.6mm	Mobile Phase A:	20mmol Ammonium Acetate
Serial No:	H22041502	Mobile Phase B:	ACN
Batch No:	H2201A	Flow Rate:	1ml/min
HPLC Column:	C18 250*4.6*5 μ m	Temperature:	Ambient
Sample:	Blank Water	Detector:	254nm

Gradient run:

Time	A%	B%
0	90	10
15	45	55
25	10	90
30	10	90
35	10	90
35.1	90	10
40	90	10

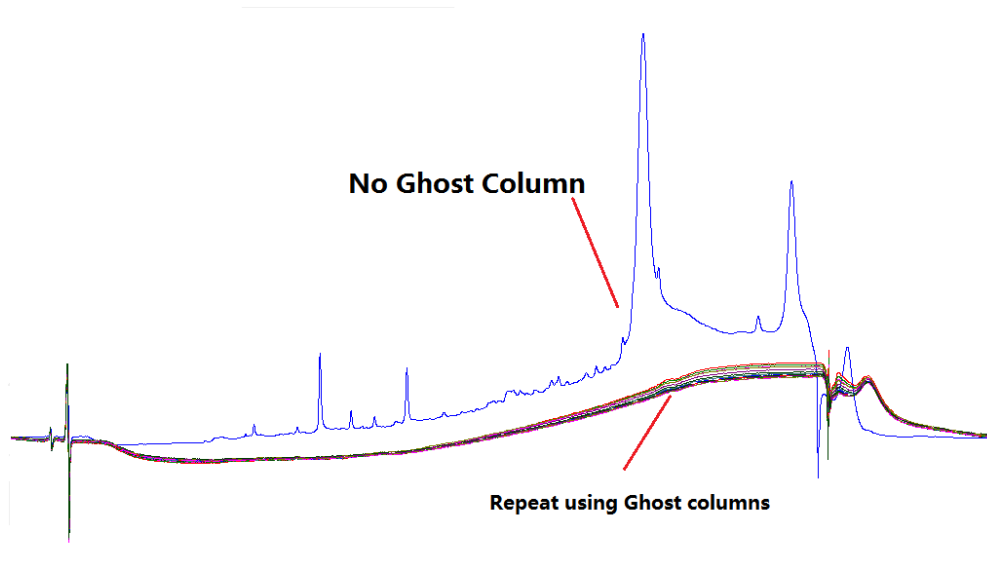

Test Result: Qualified

网址: www.hungpu.com

全国服务热线: 15112133148

