


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BH18-2110	Mobile Phase:	ACN:H2O=65:35
Serial No:	H22030302	Flow Rate:	0.45ml/min
Batch No:	Hungpu HSS T3 1.8 μ m	Temperature:	Ambient
Bulk Material:	100mm	Detector:	254nm
Dimensions:	2.1mm	Injection Volume:	1 μ l
Pressure:	10772Psi	Sample:	Acetone、Acenaphthene

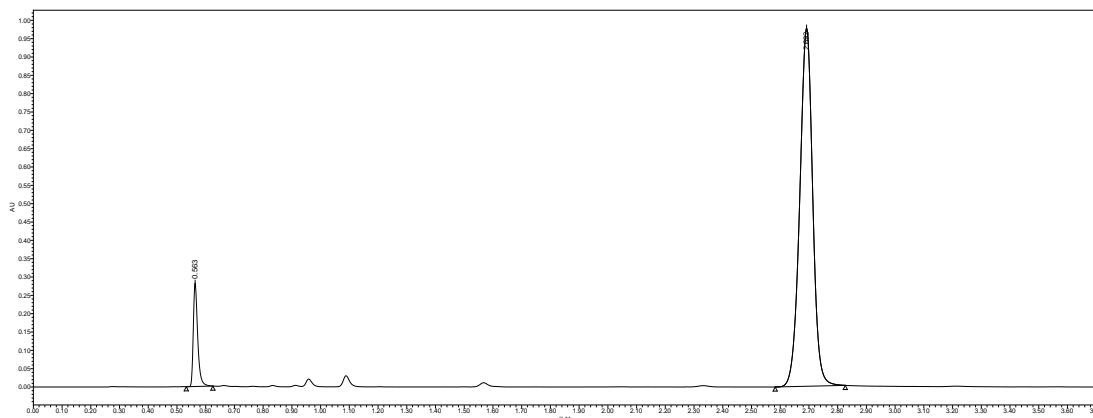

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.56	1.42	69710
2	Acenaphthene	2.69	0.96	180570

Test Result: Qualified

网址: www.hungpu.com

全国服务热线: 15112133148

