


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BH25-2105	Mobile Phase:	ACN:H2O=65:35
Serial No:	H22042702	Flow Rate:	0.45ml/min
Batch No:	HSS02025-J10-011001	Temperature:	Ambient
Bulk Material:	Hungpu HSS T3 2.5 $\mu$ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	1 $\mu$ l
Pressure:	5641Psi	Sample:	Acetone、Acenaphthene

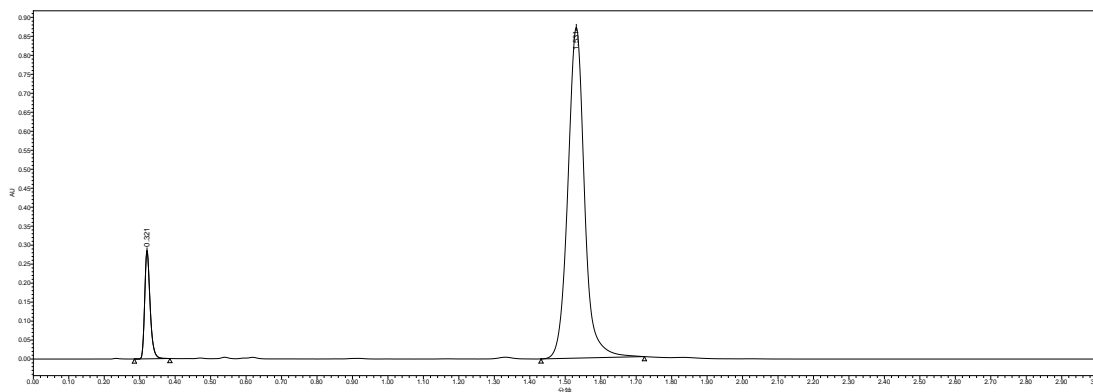

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.32	1.32	45060
2	Acenaphthene	1.53	1.06	120660

Test Result: Qualified

网址: [www.hungpu.com](http://www.hungpu.com)

全国服务热线: 15112133148

