


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BS05-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22033106	Flow Rate:	1.0ml/min
Batch No:	S02050-J01-011001	Temperature:	Ambient
Bulk Material:	Hungpu ST C18 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5 μ l
Pressure:	5.3Mpa	Sample:	Uracil 、 Acetone、 Acenaphthene

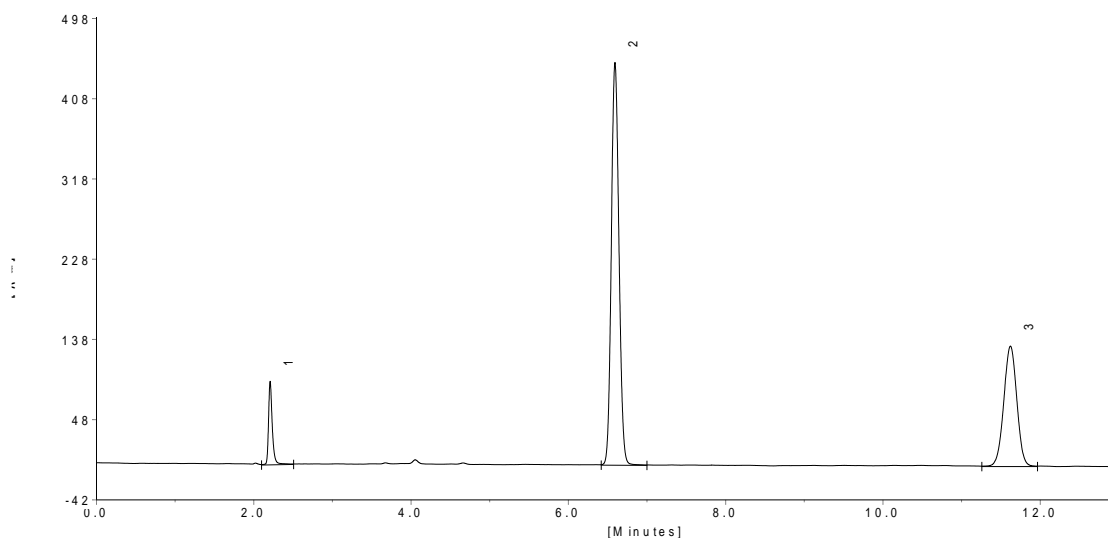

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Uracil	2.20	1.36	49585
2	Toluene	6.59	1.11	88736
3	Acenaphthene	11.62	1.00	94097

Test Result:Qualified

网址: www.hungpu.com

全国服务热线: 15112133148

