


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BA03-4615	Mobile Phase:	ACN:H2O=75:25
Serial No:	H22052801	Flow Rate:	0.8ml/min
Batch No:	D02030-J10-011001	Temperature:	Ambient
Bulk Material:	Hungpu T3 3μm	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	5μl
Pressure:	9.6Mpa	Sample:	Acetone、Acenaphthene

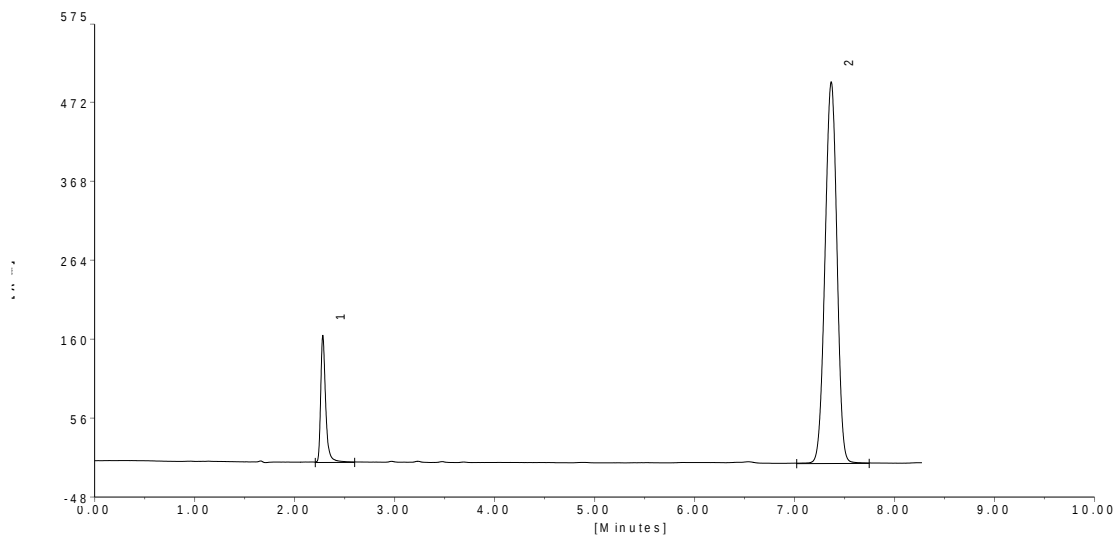

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.28	1.46	77134
2	Acenaphthene	7.30	1.04	122556

Test Result:Qualified

