


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BA05-4625	Mobile Phase:	ACN:H2O=75:25
Serial No:	H22030301	Flow Rate:	0.8ml/min
Bulk Material:	Hungpu T3 5 μ m	Temperature:	Ambient
Column Length:	250mm	Detector:	254nm
Column ID:	4.6mm	Injection Volume:	5 μ l
Pressure:	4.9Mpa	Sample:	Acetone、Acenaphthene

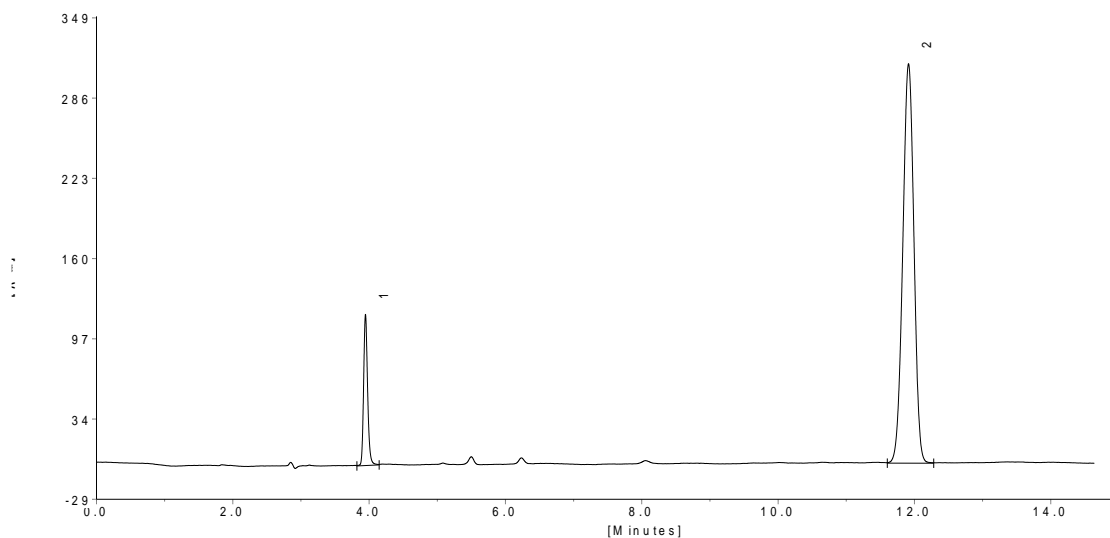

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	3.94	1.21	93231
2	Acenaphthene	11.91	0.98	99839

Test Result: Qualified

