


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BA05-4625	Mobile Phase:	ACN:H2O=75:25
Serial No:	H22050113	Flow Rate:	0.8ml/min
Batch No:	H02050-J10-011003	Temperature:	Ambient
Bulk Material:	Hungpu T3 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5 μ l
Pressure:	5.3Mpa	Sample:	Acetone、Acenaphthene

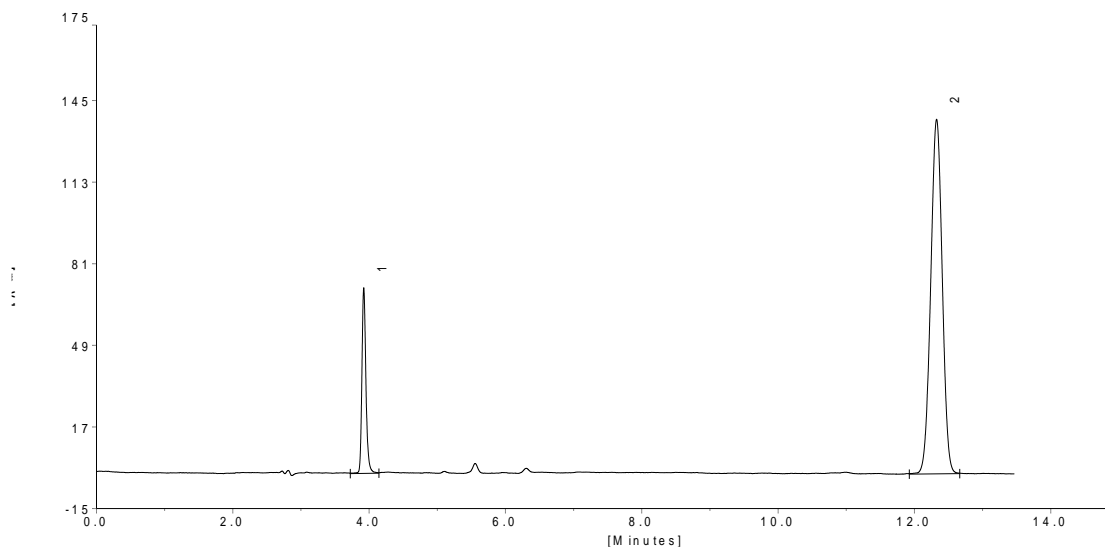

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	3.92	1.23	94628
2	Acenaphthene	12.32	1.00	102012

Test Result: Qualified

