


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX03-4610	Mobile Phase:	ACN:H2O=60:40
Serial No:	H22011704	Flow Rate:	0.8ml/min
Bulk Material:	Hungpu XBT C18 3um	Temperature:	Ambient
Column Length:	100mm	Detector:	254nm
Column ID:	4.6mm	Injection Volume:	5ul
Pressure:	1012Psi	Sample:	Uracil 、Toluene、 Acenaphthene

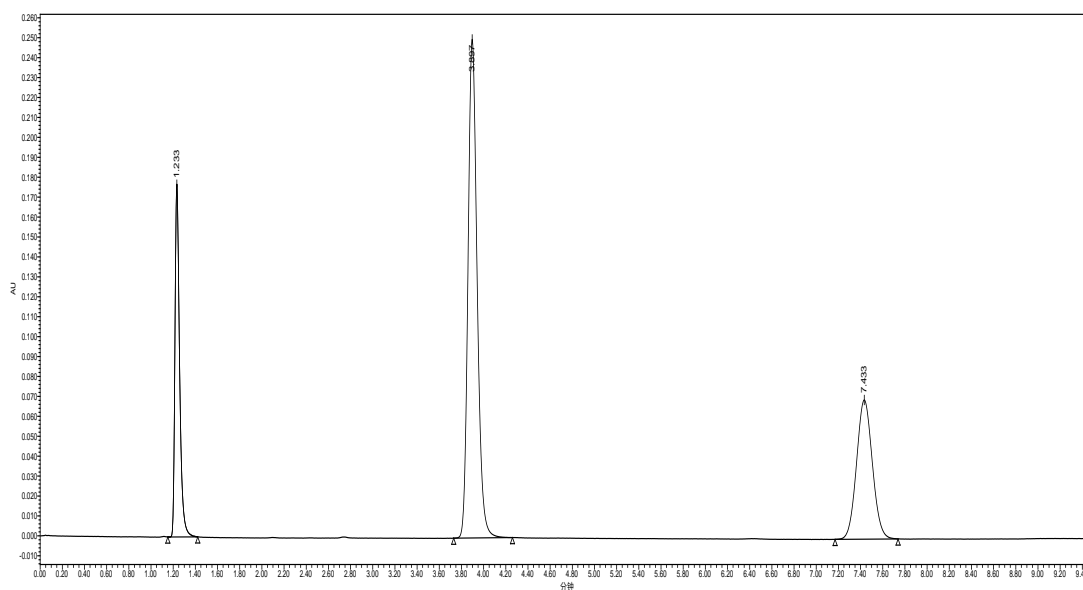

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Uracil	1.23	1.46	44388
2	Toluene	3.89	1.19	110852
3	Acenaphthene	7.43	1.06	129298

Test Result: Qualified

