


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX05-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22042402	Flow Rate:	0.8ml/min
Batch No:	H02050-J06-011005	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 5 $\mu$ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5 $\mu$ l
Pressure:	5.9Mpa	Sample:	Acetone、Acenaphthene

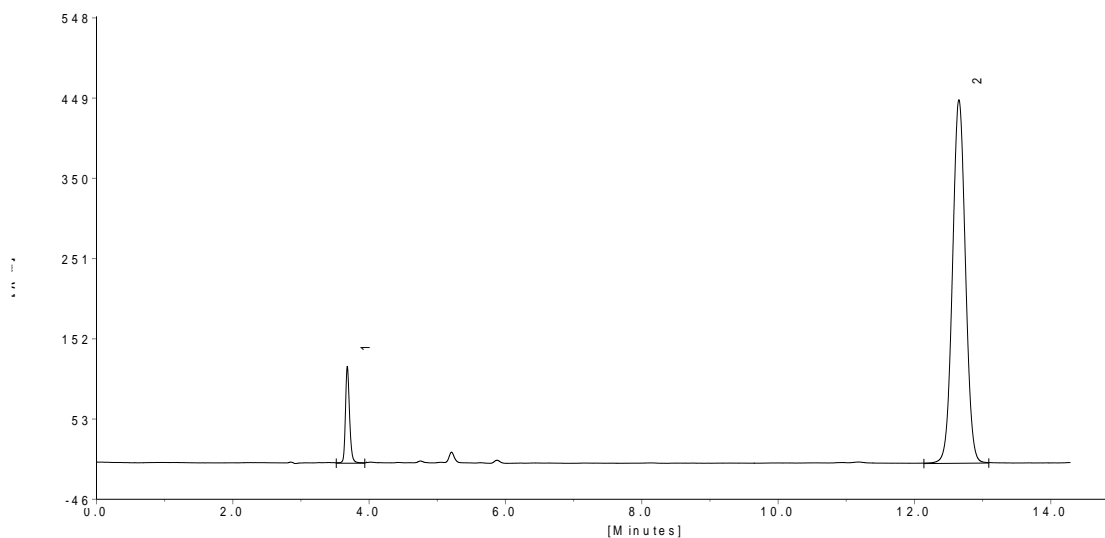

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	3.67	1.24	78880
2	Acenaphthene	12.65	1.03	85814

Test Result:Qualified

