


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX25-2105	Mobile Phase:	ACN:H2O=60:40
Serial No:	H22050104	Flow Rate:	0.2ml/min
Batch No:	H02025-J06-011001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 2.5 μ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	1 μ l
Pressure:	1730Psi	Sample:	Acetone、Acenaphthene

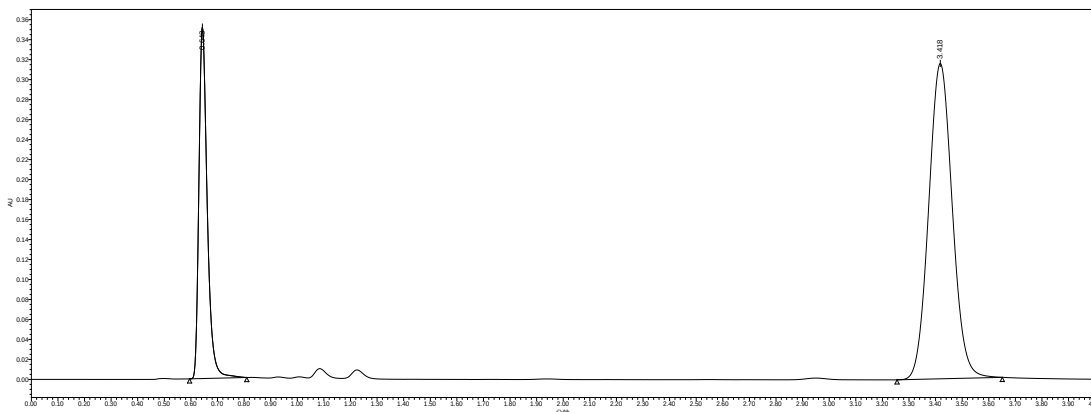

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.64	1.38	43060
2	Acenaphthene	3.41	1.06	142100

Test Result:Qualified

