


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BXT5-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22052701	Flow Rate:	0.8ml/min
Batch No:	HG02050-J10-011004	Temperature:	Ambient
Bulk Material:	Hungpu XBT T3 5μm	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	5μl
Pressure:	4.7Mpa	Sample:	Acetone、Acenaphthene

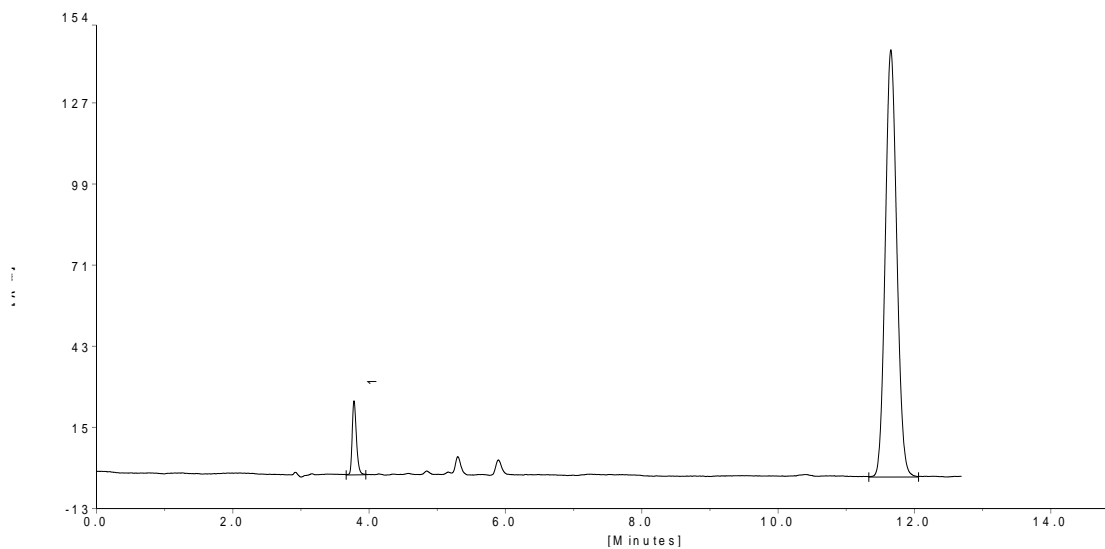

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	3.77	1.30	74876
2	Acenaphthene	11.65	1.09	91197

Test Result:Qualified

