


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-WT05-2110	Mobile Phase:	ACN:H2O=60:40
Serial No:	H22041703	Flow Rate:	0.2ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C4-300 5 μ m	Detector:	254nm
Dimensions:	100*2.1mm	Injection Volume:	0.2 μ l
Pressure:	62bar	Sample:	Toluene

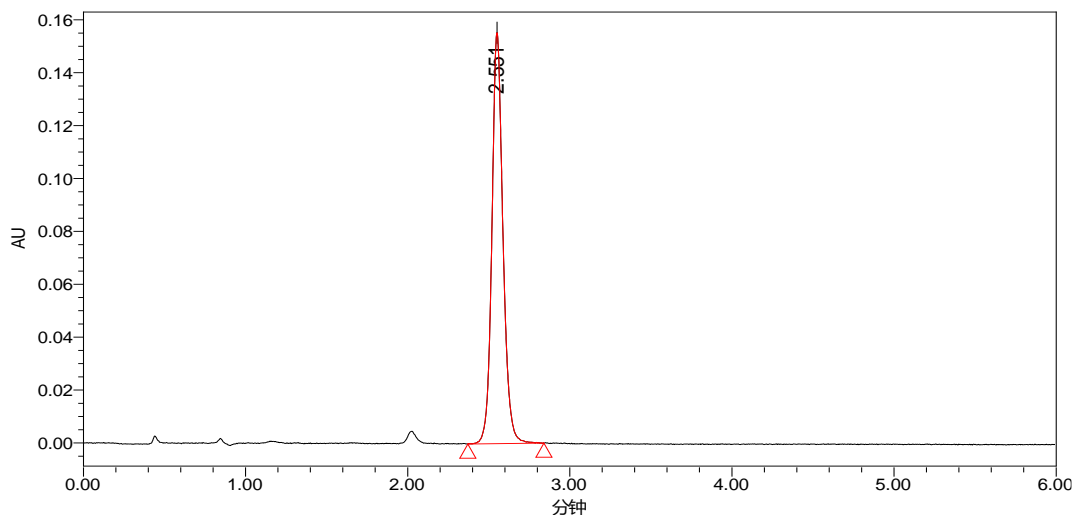

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	2.55	1.1	7134

Test Result: Qualified

