


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-4615	Mobile Phase:	MeOH:H2O=75:25
Serial No:	H22041401	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase	Hungpu C18-AQ(2) 3 $\mu$ m	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	20 $\mu$ l
Pressure:	206bar	Sample:	Toluene

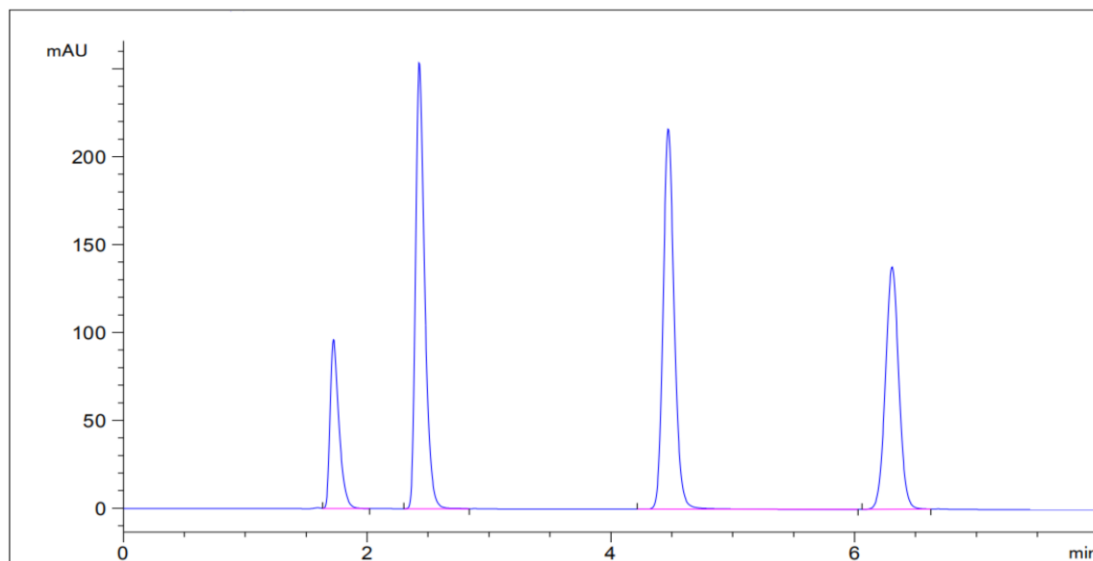

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	6.239	1.04	18354

Test Result: Qualified

