


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-X10-2025	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22061902	Flow Rate:	20ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ 10 μ m	Detector:	254nm
Dimensions:	250*20mm	Injection Volume:	200 μ l
Pressure:	15bar	Sample:	Toluene

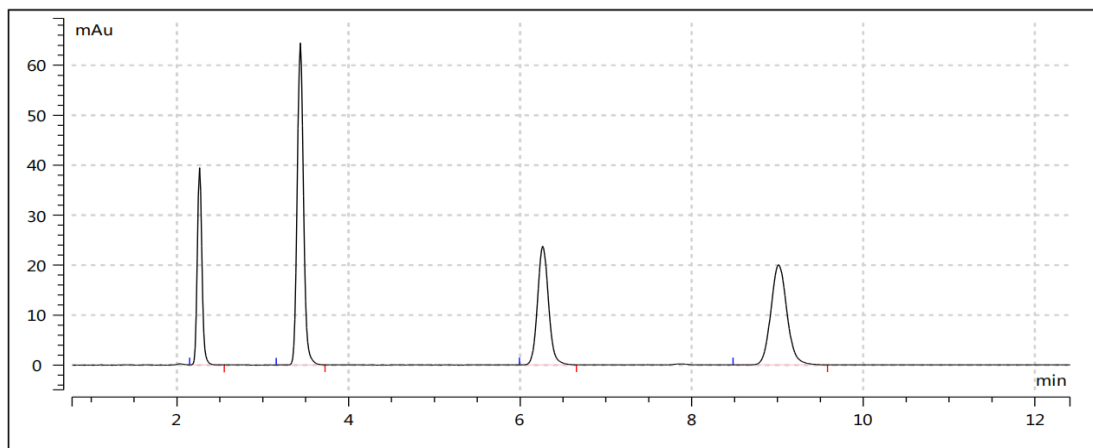

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	9.014	1.10	11511

Test Result: Qualified

