


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-0310	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22062701	Flow Rate:	0.6ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ(2) 3 μ m	Detector:	254nm
Dimensions:	100*3.0mm	Injection Volume:	10 μ l
Pressure:	101bar	Sample:	Toluene

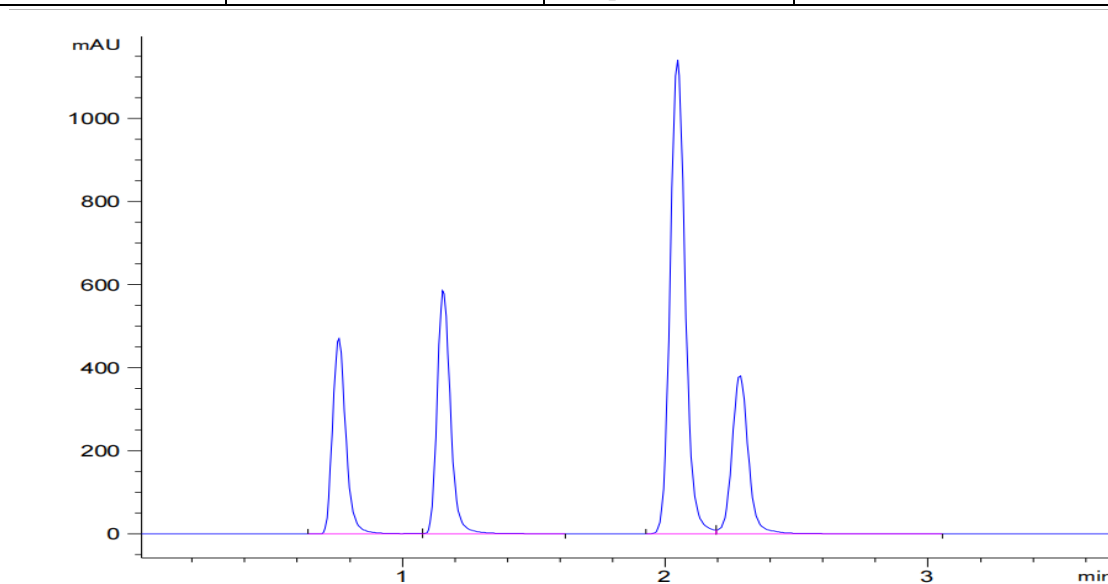

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	2.284	1.05	6781

Test Result: Qualified

