


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-4625	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22070302	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ(2) 3 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	10 μ l
Pressure:	172bar	Sample:	Toluene

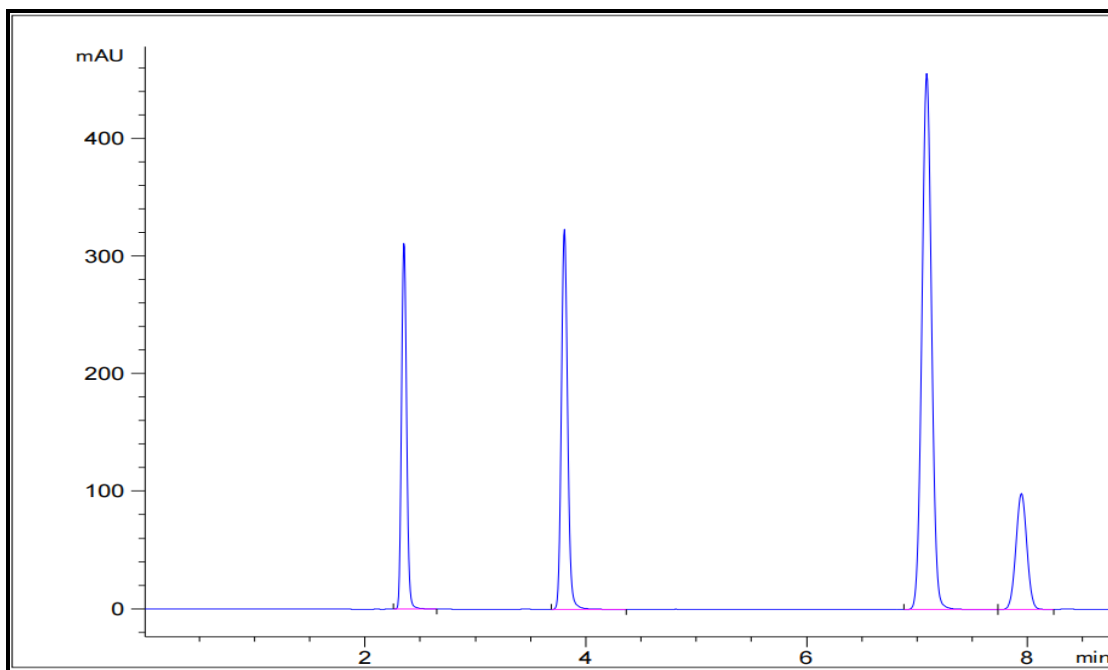

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	7.946	1.01	30747

Test Result: Qualified

