


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-C05-4125	Mobile Phase:	MeOH:H <sub>2</sub> O=75:25
Serial No:	H22061101	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Stationary Phase:	Hungpu C8 5 $\mu$ m	Detector:	254nm
Dimensions:	125*4.0mm	Injection Volume:	100 $\mu$ l
Pressure:	67bar	Sample:	Toluene

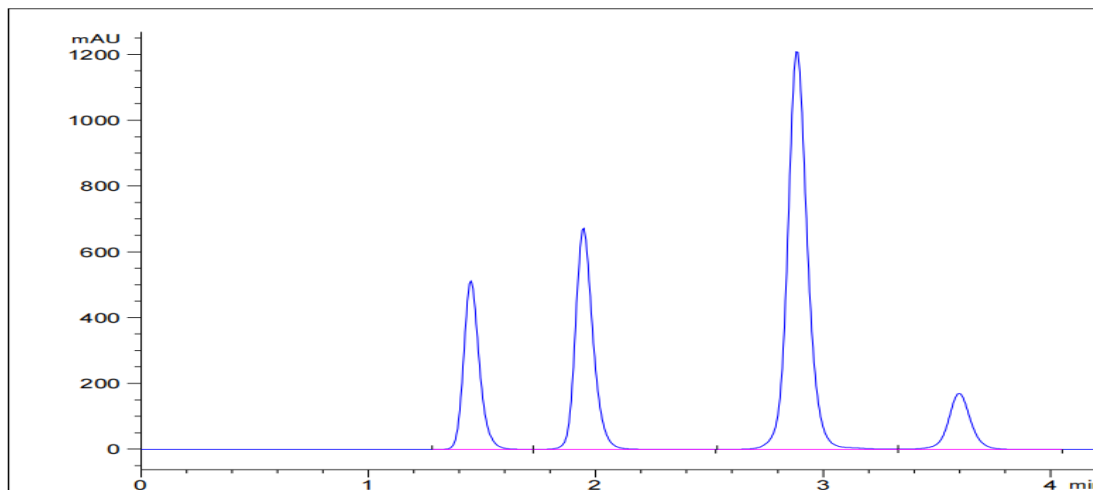

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	3.647	1.04	7247

Test Result: Qualified

