


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-J05-4625	Mobile Phase:	ACN:H2O=30:70
Serial No:	H22062702	Flow Rate:	1ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu CN 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	20 μ l
Pressure:	94bar	Sample:	Tetrachloronitrobenzene

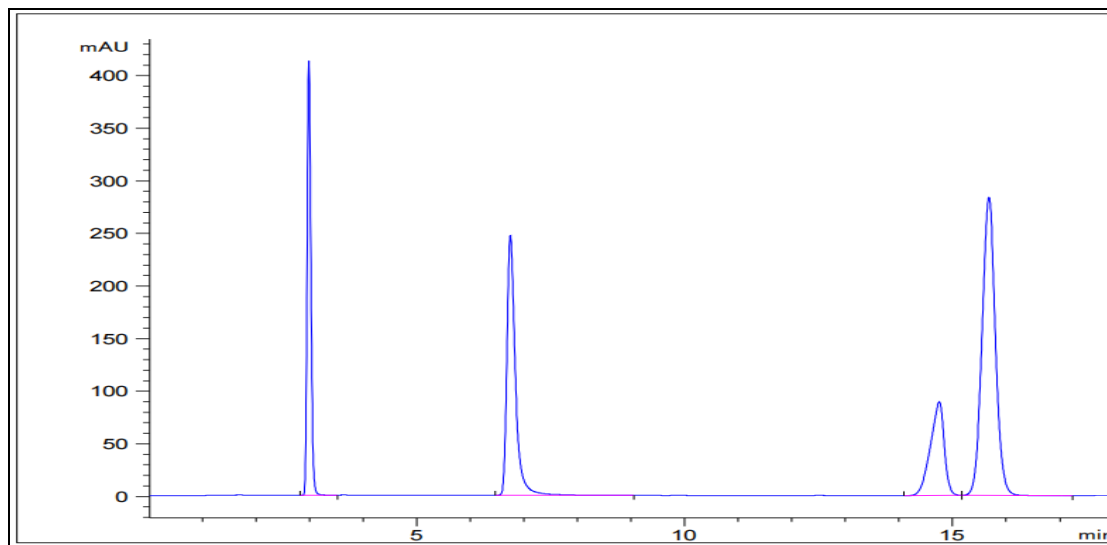

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Tetrachloronitro benzene	15.677	1.02	19401

Test Result: Qualified

