


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BS05-4615	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22061703	Flow Rate:	0.8ml/min
Batch No:	S02050-J01-011002	Temperature:	Ambient
Bulk Material:	Hungpu ST C18 5 μ m	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	5 μ l
Pressure:	3.7Mpa	Sample:	Acetone、Acenaphthene

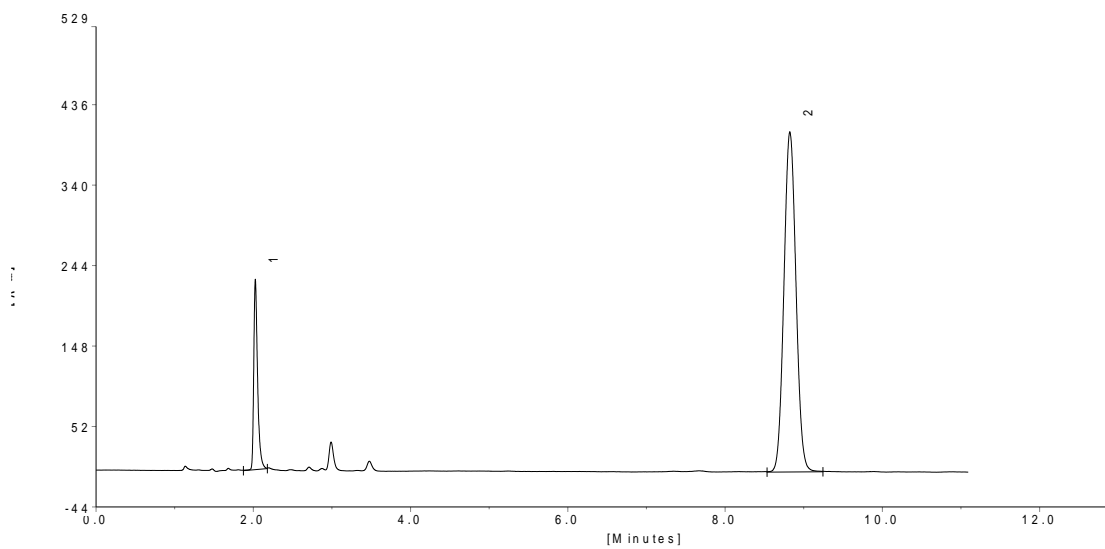

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.02	1.47	62754
2	Acenaphthene	8.82	1.07	104553

Test Result: Qualified

