


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX03-4615	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22060501	Flow Rate:	0.8ml/min
Batch No:	HG02030-J06-011002	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 3 μ m	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	5 μ l
Pressure:	7.1Mpa	Sample:	Acetone、Acenaphthene

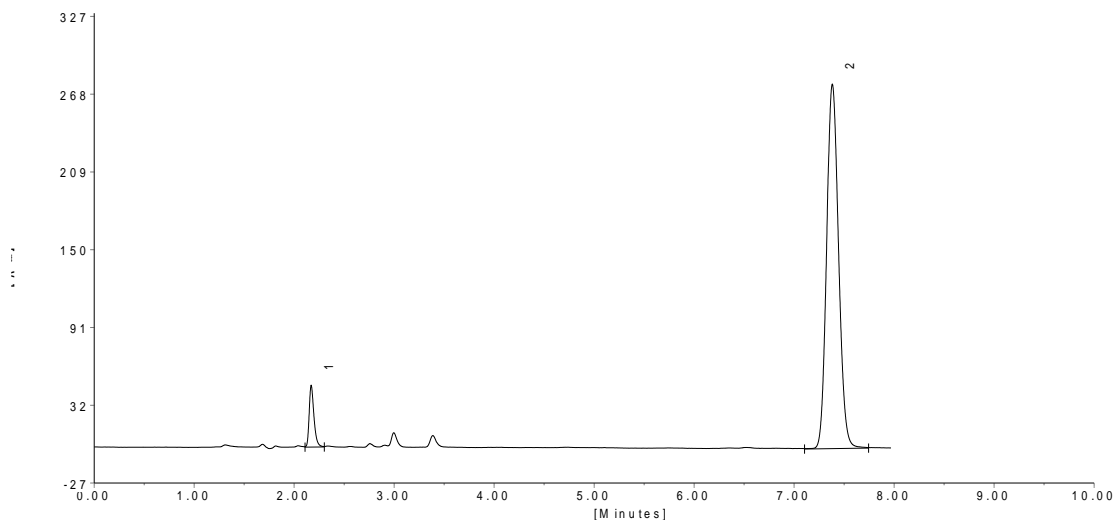

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.17	1.39	74446
2	Acenaphthene	7.38	1.10	122193

Test Result: Qualified

