


## HPLC COLUMN TEST SUMMARY

|                |                    |                   |                      |
|----------------|--------------------|-------------------|----------------------|
| Catalog No:    | HP-BX03-4615       | Mobile Phase:     | ACN:H2O=70:30        |
| Serial No:     | H22060502          | Flow Rate:        | 0.8ml/min            |
| Batch No:      | HG02030-J06-011002 | Temperature:      | Ambient              |
| Bulk Material: | Hungpu XBT C18 3μm | Detector:         | 254nm                |
| Dimensions:    | 150*4.6mm          | Injection Volume: | 5μl                  |
| Pressure:      | 7.1Mpa             | Sample:           | Acetone、Acenaphthene |

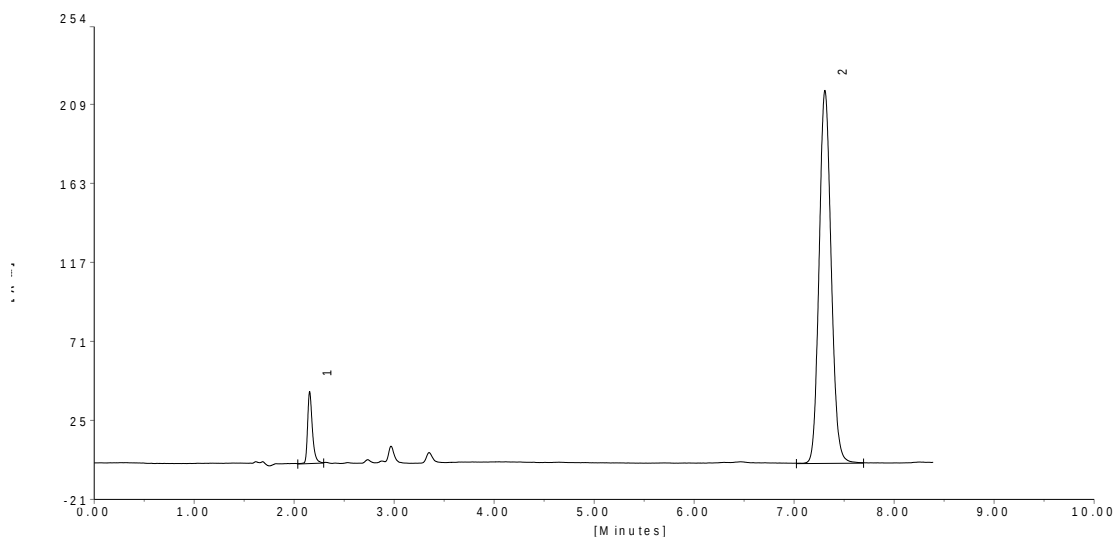

| Item | Sample       | Ret Time<br>(min) | USP Tailing<br>(As) | Efficiency<br>(N/m) |
|------|--------------|-------------------|---------------------|---------------------|
| 1    | Acetone      | 2.15              | 1.38                | 71062               |
| 2    | Acenaphthene | 7.32              | 1.10                | 123212              |

Test Result:Qualified

