


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX03-4615	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22060503	Flow Rate:	0.8ml/min
Batch No:	HG02030-J06-011002	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 3 $\mu$ m	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	5 $\mu$ l
Pressure:	6.9Mpa	Sample:	Acetone、Acenaphthene

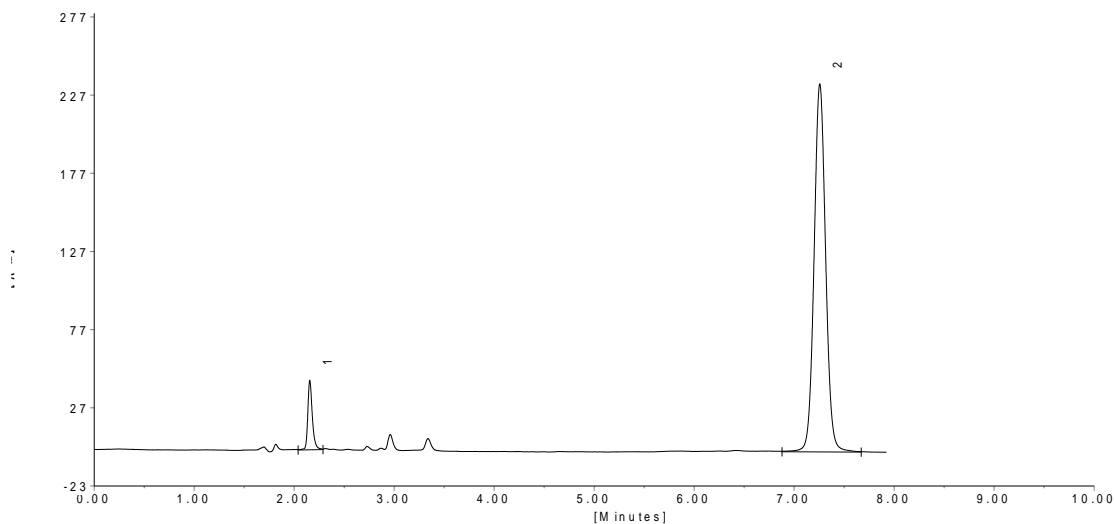

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	2.15	1.32	84766
2	Acenaphthene	7.25	1.06	131355

Test Result: Qualified

