


HPLC COLUMN TEST SUMMARY

| | | | |
|----------------|----------------------------|-------------------|----------------------|
| Catalog No: | HP-BX25-2105 | Mobile Phase: | ACN:H2O=50:50 |
| Serial No: | H22061207 | Flow Rate: | 0.6ml/min |
| Batch No: | H02025-J06-011001 | Temperature: | Ambient |
| Bulk Material: | Hungpu XBT C18 2.5 μ m | Detector: | 254nm |
| Dimensions: | 50*2.1mm | Injection Volume: | 1 μ l |
| Pressure: | 5087Psi | Sample: | Acetone、Acenaphthene |

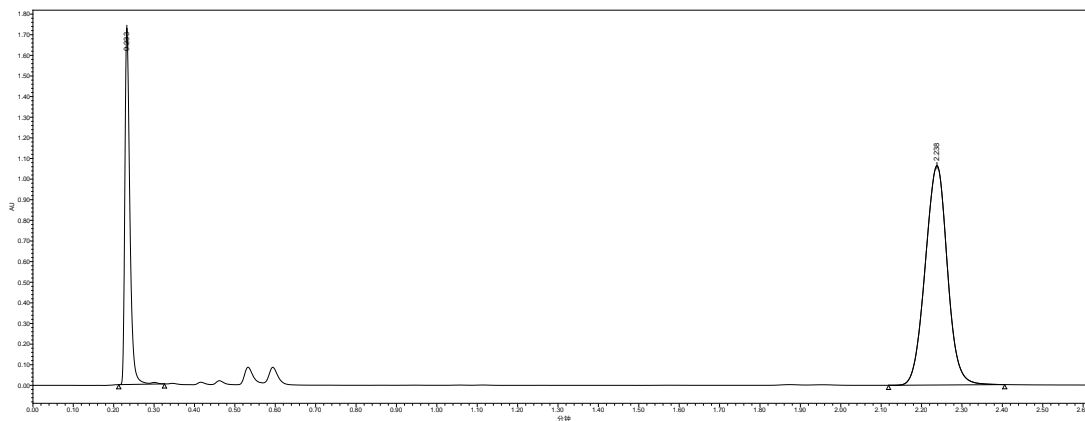

| Item | Sample | Ret Time (min) | USP Tailing (As) | Efficiency (N/m) |
|------|--------------|-------------------|---------------------|---------------------|
| 1 | Acetone | 0.23 | 1.47 | 36340 |
| 2 | Acenaphthene | 2.23 | 1.00 | 161300 |

Test Result:Qualified

