


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BX25-2105	Mobile Phase:	ACN:H2O=50:50
Serial No:	H22061209	Flow Rate:	0.6ml/min
Batch No:	H02025-J06-011001	Temperature:	Ambient
Bulk Material:	Hungpu XBT C18 2.5 $\mu$ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	1 $\mu$ l
Pressure:	5092Psi	Sample:	Acetone、Acenaphthene

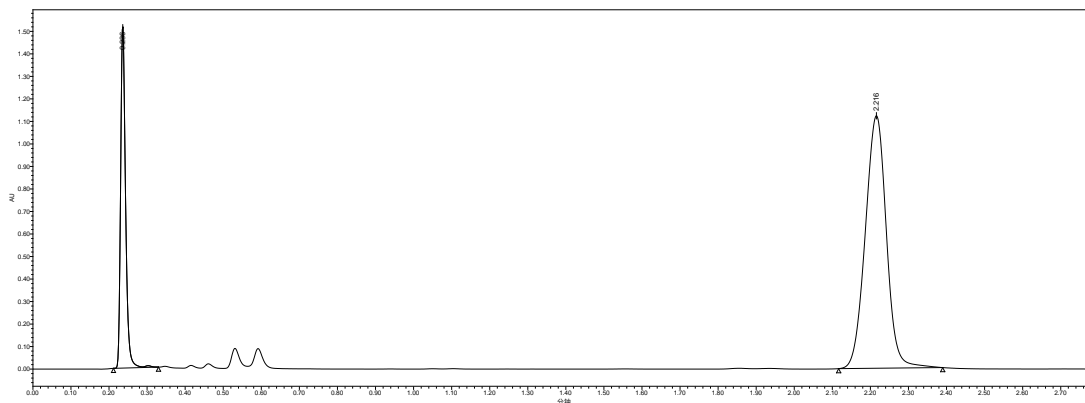

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.23	1.29	33460
2	Acenaphthene	2.21	0.98	156760

Test Result: Qualified

