


HPLC COLUMN TEST SUMMARY

| | | | |
|----------------|----------------------|-------------------|---------------|
| Catalog No: | HP-B03-0410 | Mobile Phase: | ACN:H2O=70:30 |
| Serial No: | H22070401 | Flow Rate: | 0.8ml/min |
| Batch No: | H2201A | Temperature: | Ambient |
| Bulk Material: | Hungpu C18 3 μ m | Detector: | 254nm |
| Dimensions: | 100*4.0mm | Injection Volume: | 10 μ l |
| Pressure: | 94bar | Sample: | Toluene |

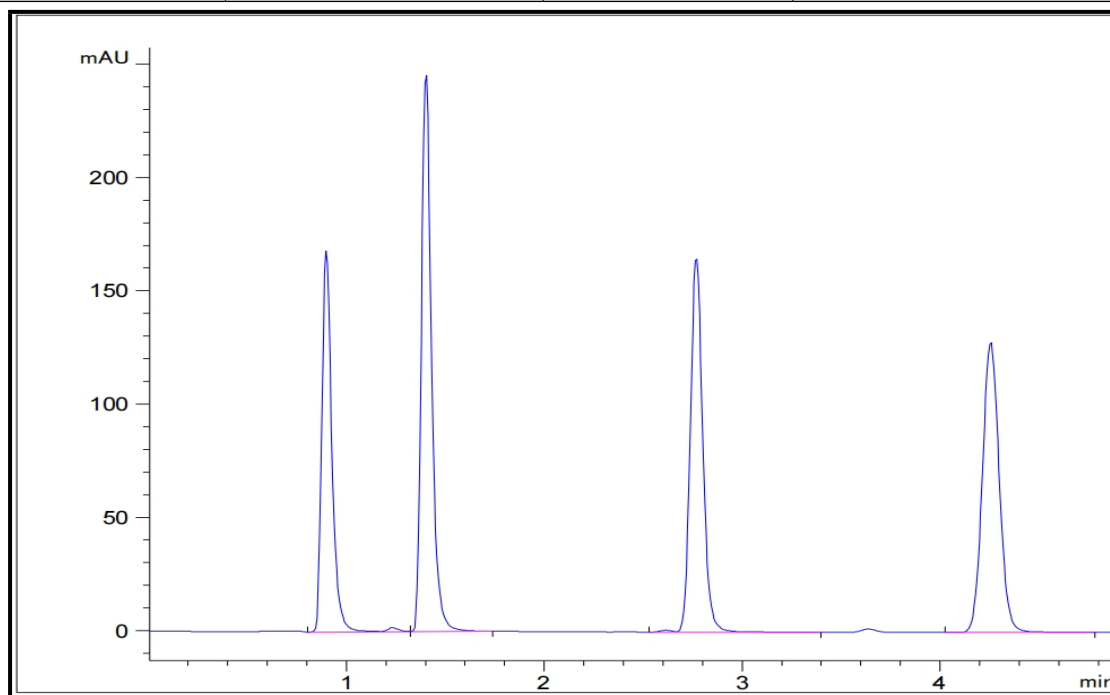

| Item | Sample | Ret Time (min) | USP Tailing (As) | Efficiency (N/m) |
|------|---------|-------------------|---------------------|---------------------|
| 1 | Toluene | 4.256 | 1.04 | 12162 |

Test Result: Qualified

