


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-0315	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22072801	Flow Rate:	1.0ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ(2) 3 μ m	Detector:	254nm
Dimensions:	150*3.0mm	Injection Volume:	10 μ l
Pressure:	146bar	Sample:	Toluene

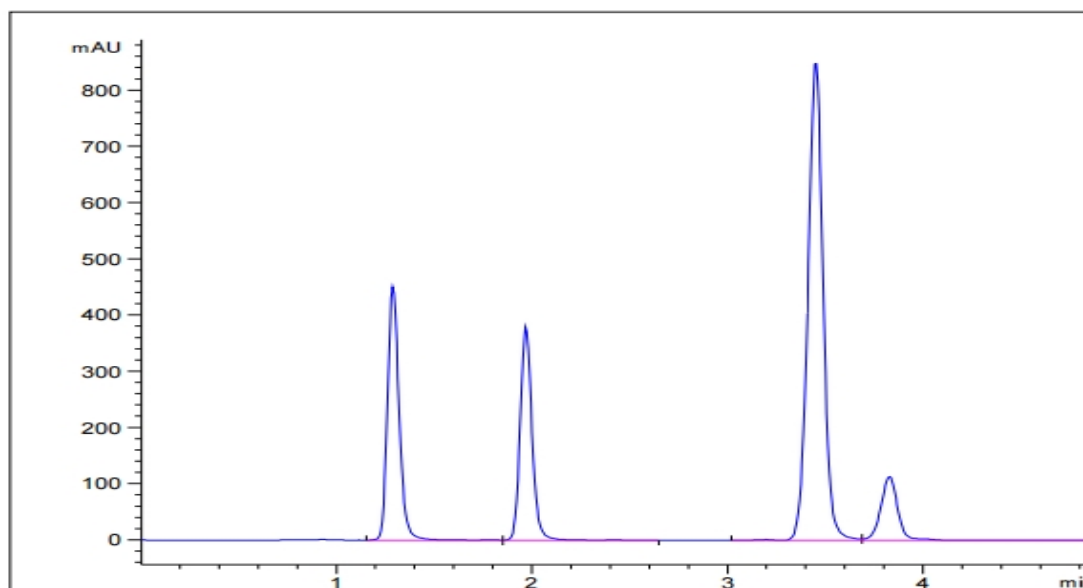

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Toluene	3.829	0.98	10415

Test Result: Qualified

