


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-Y03-4615	Mobile Phase:	MeOH:H <sub>2</sub> O=75:25
Serial No:	H22080401	Flow Rate:	1.0ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C18-AQ(2) 3μm	Detector:	254nm
Dimensions:	150*4.6mm	Injection Volume:	20μl
Pressure:	196bar	Sample:	Toluene

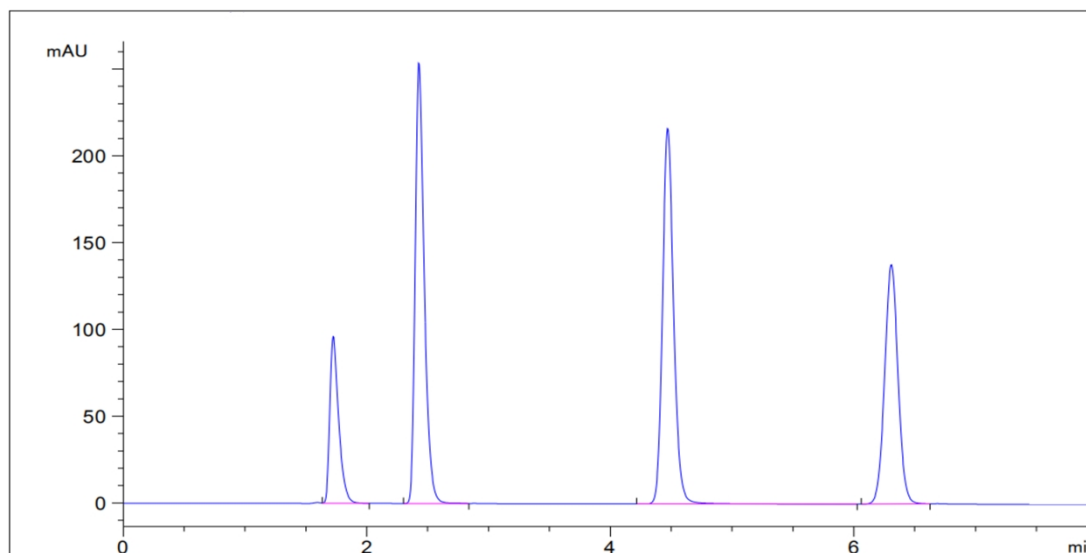

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N)
1	Toluene	6.239	1.02	15829

Test Result:Qualified

