


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-T05-4625	Mobile Phase:	MeOH:H ₂ O=75:25
Serial No:	H22073102	Flow Rate:	1.0ml/min
Batch No:	H2201A	Temperature:	Ambient
Bulk Material:	Hungpu C30 5 μ m	Detector:	254nm
Dimensions:	250*4.6mm	Injection Volume:	20 μ l
Pressure:	130bar	Sample:	Toluene

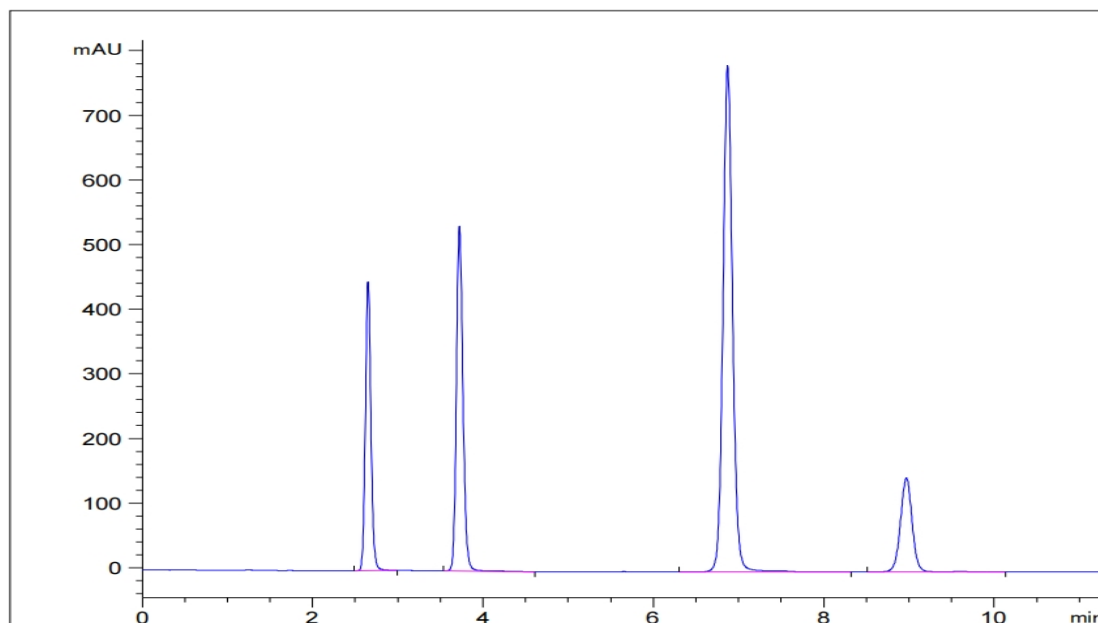

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N)
1	Toluene	8.963	1.00	22497

Test Result: Qualified

