


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BH18-2110	Mobile Phase:	ACN:H2O=65:35
Serial No:	H22030302	Flow Rate:	0.45ml/min
Batch No:	HSS02018-J10-011001	Temperature:	Ambient
Bulk Material:	Hungpu HSS T3 2.5 μ m	Detector:	254nm
Dimensions:	100*2.1mm	Injection Volume:	1 μ l
Pressure:	10560Psi	Sample:	Acetone、Acenaphthene

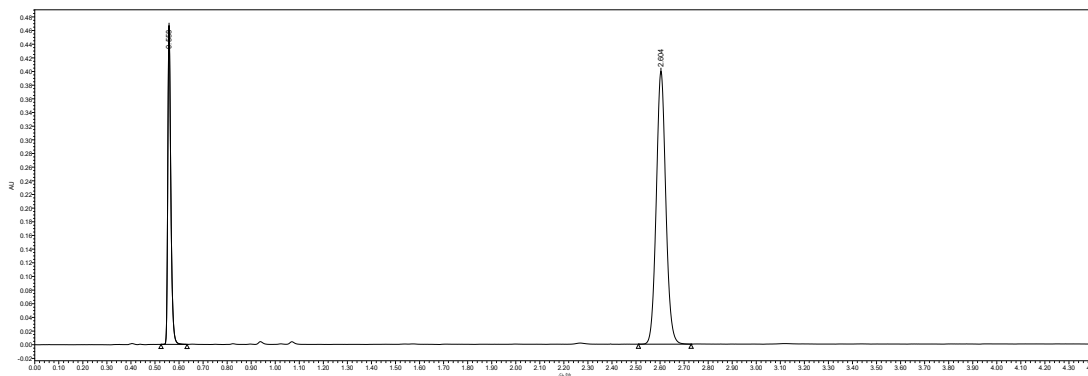

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.55	1.40	98450
2	Acenaphthene	2.60	1.07	211070

Test Result:Qualified

