


HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BH25-2110	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22072414	Flow Rate:	0.3ml/min
Batch No:	HSS02025-J10-012001	Temperature:	Ambient
Bulk Material:	Hungpu HSS T3 2.5 μ m	Detector:	254nm
Dimensions:	100*2.1mm	Injection Volume:	1 μ l
Pressure:	3332Psi	Sample:	Acetone、Acenaphthene

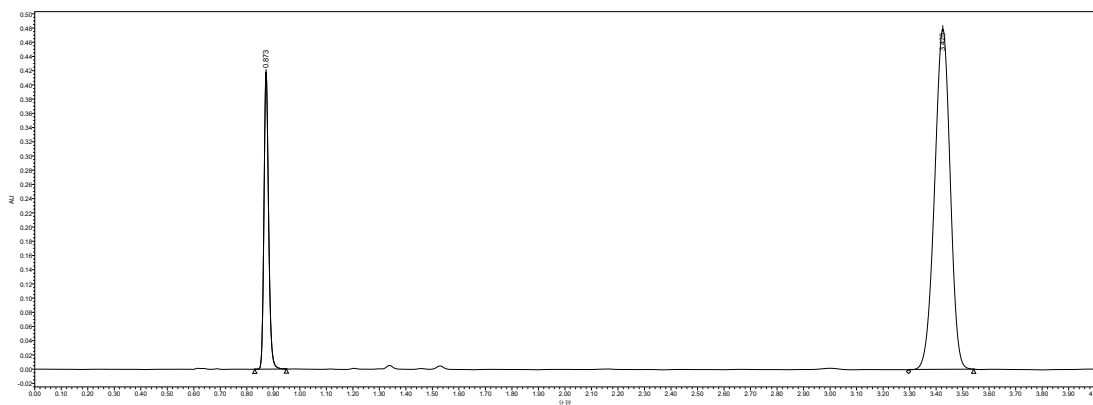

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.87	1.19	123990
2	Acenaphthene	3.42	0.95	160780

Test Result:Qualified

