


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BH25-2105	Mobile Phase:	ACN:H2O=70:30
Serial No:	H22072102	Flow Rate:	0.3ml/min
Batch No:	HSS02025-J10-012001	Temperature:	Ambient
Bulk Material:	Hungpu HSS T3 2.5 $\mu$ m	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	1 $\mu$ l
Pressure:	1886Psi	Sample:	Acetone、Acenaphthene

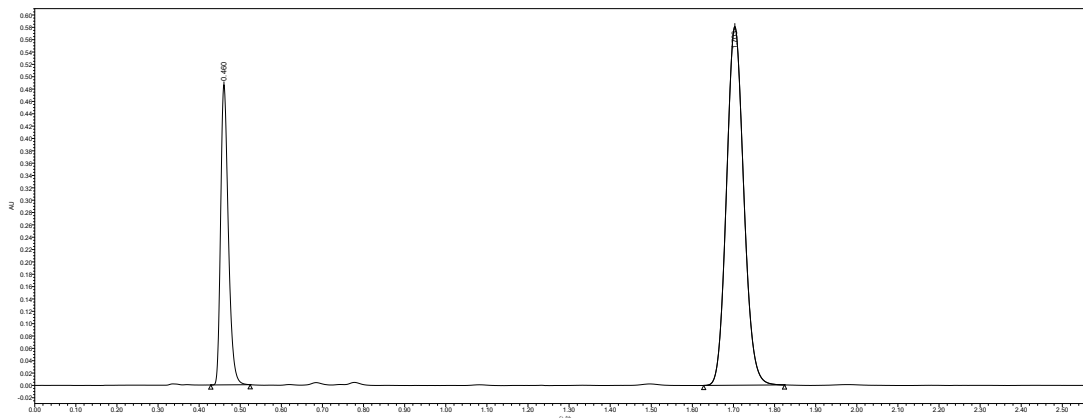

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.46	1.32	58760
2	Acenaphthene	1.70	1.10	157200

Test Result: Qualified

