


HPLC COLUMN TEST SUMMARY

| | | | |
|----------------|---------------------------|-------------------|----------------------|
| Catalog No: | HP-BH25-2105 | Mobile Phase: | ACN:H2O=70:30 |
| Serial No: | H22073003 | Flow Rate: | 0.3ml/min |
| Batch No: | HSS02025-J10-012001 | Temperature: | Ambient |
| Bulk Material: | Hungpu HSS T3 2.5 μ m | Detector: | 254nm |
| Dimensions: | 50*2.1mm | Injection Volume: | 1 μ l |
| Pressure: | 2136Psi | Sample: | Acetone、Acenaphthene |

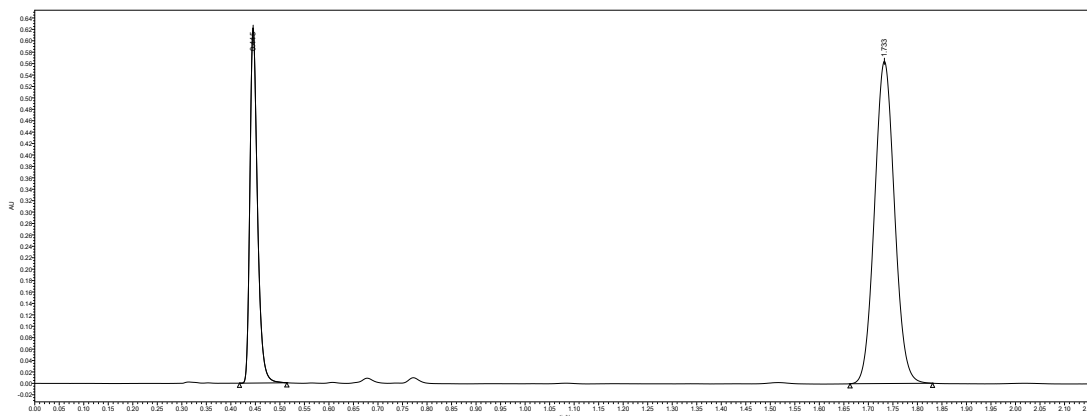

| Item | Sample | Ret Time (min) | USP Tailing (As) | Efficiency (N/m) |
|------|--------------|-------------------|---------------------|---------------------|
| 1 | Acetone | 0.44 | 1.35 | 83340 |
| 2 | Acenaphthene | 1.73 | 1.06 | 172220 |

Test Result: Qualified

