


## HPLC COLUMN TEST SUMMARY

|                |                           |                   |                      |
|----------------|---------------------------|-------------------|----------------------|
| Catalog No:    | HP-BH25-2105              | Mobile Phase:     | ACN:H2O=70:30        |
| Serial No:     | H22073004                 | Flow Rate:        | 0.3ml/min            |
| Batch No:      | HSS02025-J10-012001       | Temperature:      | Ambient              |
| Bulk Material: | Hungpu HSS T3 2.5 $\mu$ m | Detector:         | 254nm                |
| Dimensions:    | 50*2.1mm                  | Injection Volume: | 1 $\mu$ l            |
| Pressure:      | 2100Psi                   | Sample:           | Acetone、Acenaphthene |

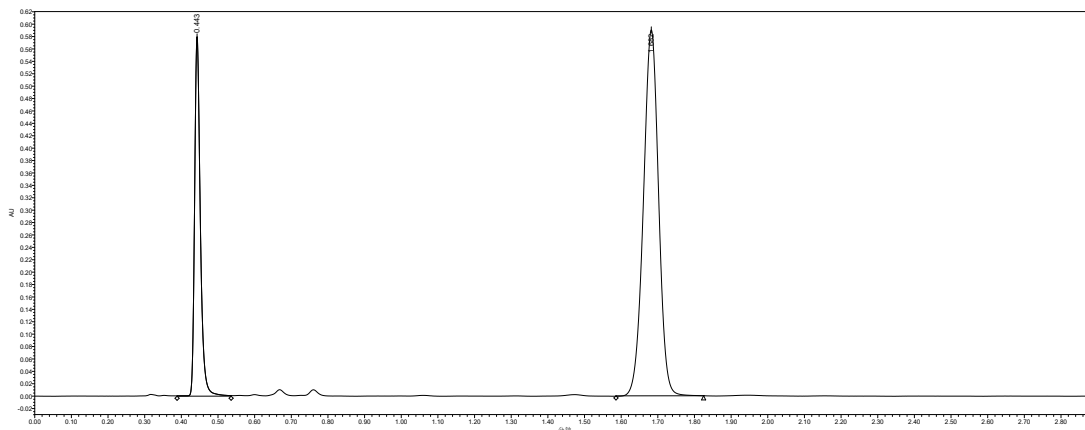

| Item | Sample       | Ret Time<br>(min) | USP Tailing<br>(As) | Efficiency<br>(N/m) |
|------|--------------|-------------------|---------------------|---------------------|
| 1    | Acetone      | 0.44              | 1.34                | 83180               |
| 2    | Acenaphthene | 1.68              | 0.97                | 159460              |

Test Result:Qualified

