


## HPLC COLUMN TEST SUMMARY

Catalog No:	HP-BH25-2105	Mobile Phase:	ACN:H <sub>2</sub> O=70:30
Serial No:	H22080506	Flow Rate:	0.3ml/min
Batch No:	HSS02025-J10-012001	Temperature:	Ambient
Bulk Material:	Hungpu HSS T3 2.5μm	Detector:	254nm
Dimensions:	50*2.1mm	Injection Volume:	1μl
Pressure:	2138Psi	Sample:	Acetone、Acenaphthene

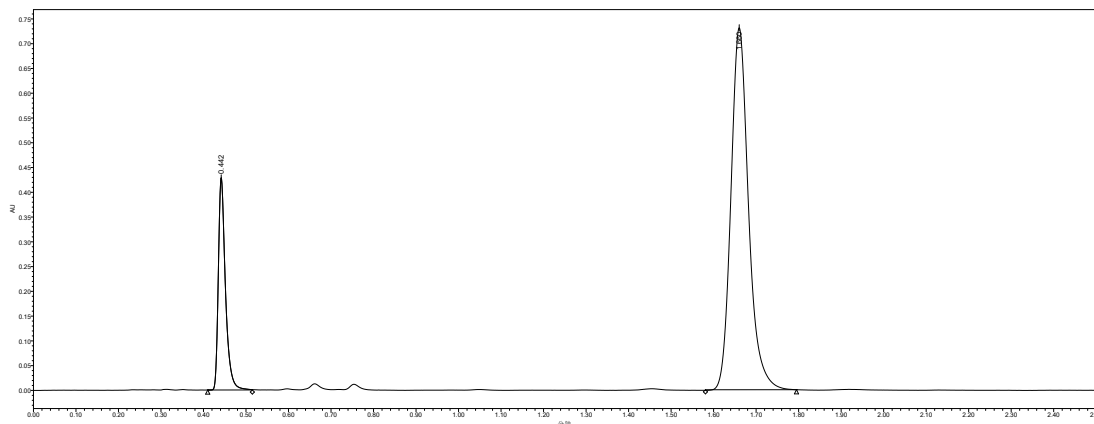

Item	Sample	Ret Time (min)	USP Tailing (As)	Efficiency (N/m)
1	Acetone	0.44	1.48	72420
2	Acenaphthene	1.66	1.18	163840

Test Result: Qualified

